

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
 Data File : BM020731.D
 Acq On : 05 Jun 2019 11:54
 Operator : HP/JU
 Sample : PB191779BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119779BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	8	13	19	rVB	244340	298201	2.03%	0.322%
2	5.404	404	411	422	rBV	5741522	8340290	56.79%	9.015%
3	6.987	672	680	697	rBV	5833589	9061219	61.70%	9.794%
4	7.357	734	743	752	rBV	5816586	9209183	62.71%	9.954%
5	7.822	814	822	832	rVB	1200750	1871489	12.74%	2.023%
6	8.140	867	876	884	rBV	4348946	7031828	47.88%	7.601%
7	8.981	1012	1019	1028	rBV	3244993	5452469	37.13%	5.894%
8	10.610	1288	1296	1305	rBV	1436266	2452122	16.70%	2.651%
9	13.080	1708	1716	1731	rBV	8541771	12587515	85.72%	13.606%
10	14.457	1944	1950	1966	rBV2	2002669	3083790	21.00%	3.333%
11	15.945	2197	2203	2220	rBV	5591844	7902117	53.81%	8.542%
12	17.204	2409	2417	2429	rBV	2385851	3405579	23.19%	3.681%
13	19.827	2857	2863	2870	rBV	12313883	14685054	100.00%	15.873%
14	21.380	3122	3127	3133	rBV	2745352	3458098	23.55%	3.738%
15	23.668	3509	3516	3526	rBV	1919335	3674944	25.03%	3.972%


Sum of corrected areas: 92513898

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
Data File : BM020731.D
Acq On : 05 Jun 2019 11:54
Operator : HP/JU
Sample : PB191779BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
PB119779BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

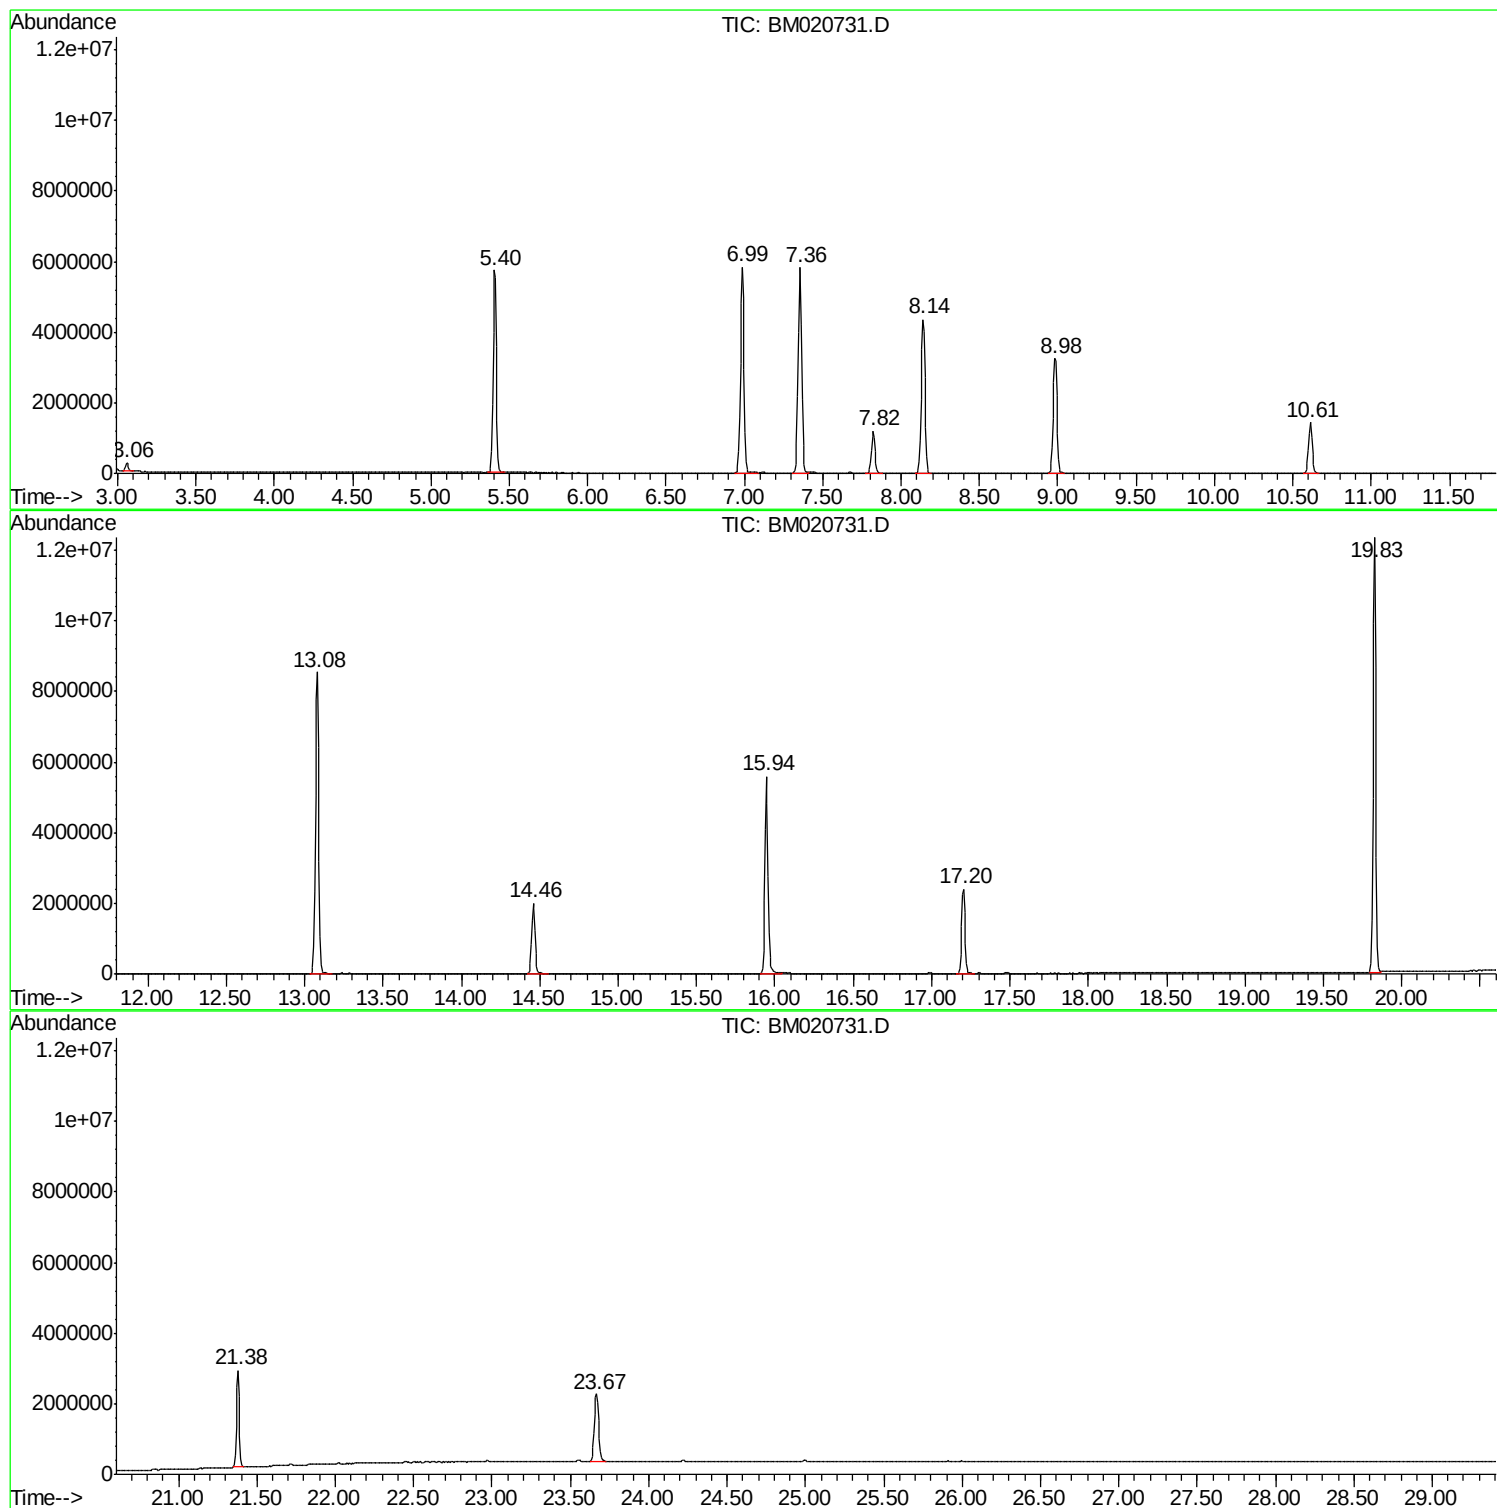

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
Data File : BM020731.D
Acq On : 05 Jun 2019 11:54
Operator : HP/JU
Sample : PB191779BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119779BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	3.19 ng	298201	1,4-Dichlorobenzene-d4	7.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	64
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	10
5		N-Ethylformamide	73	C3H7NO	000627-45-2	9

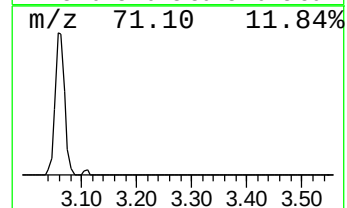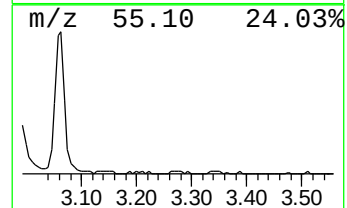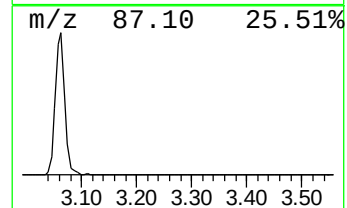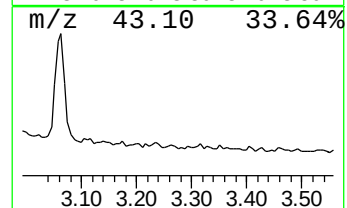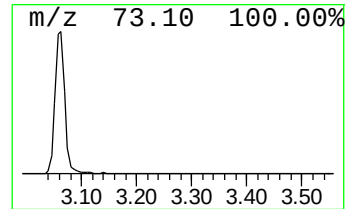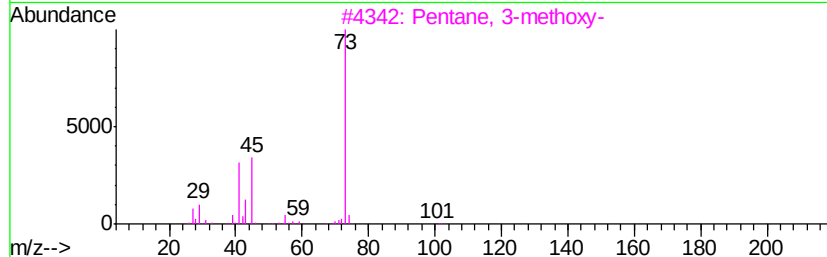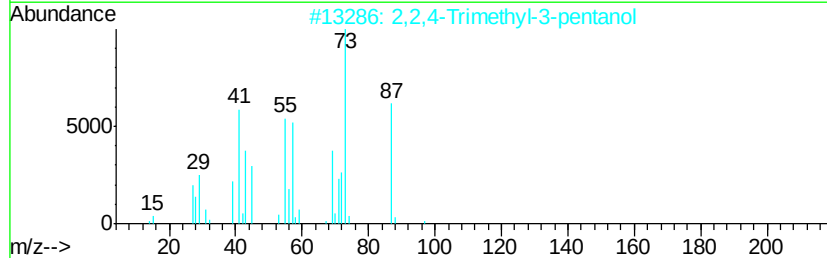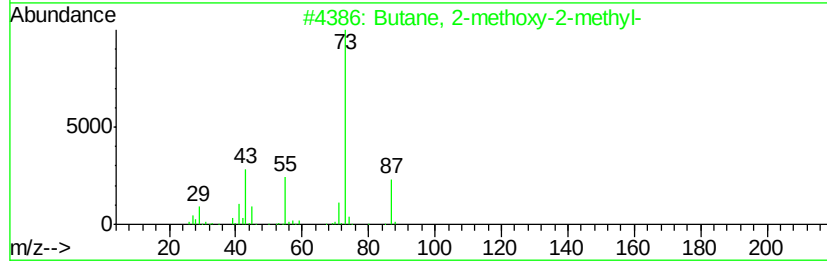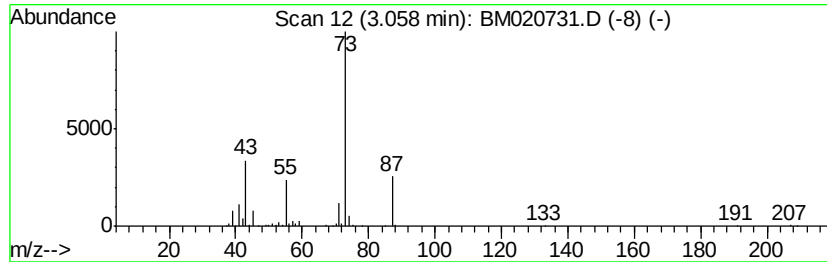

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
Data File : BM020731.D
Acq On : 05 Jun 2019 11:54
Operator : HP/JU
Sample : PB191779BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119779BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.36 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.36	98.42 ng	9209180	1,4-Dichlorobenzene-d4	7.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		Xenon	132	Xe	007440-63-3	9
4		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

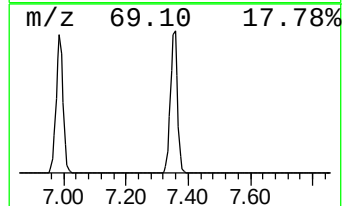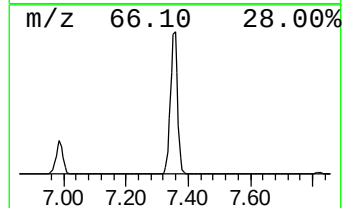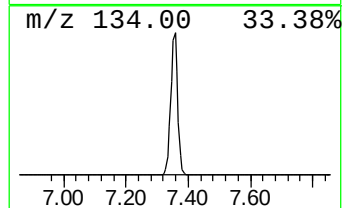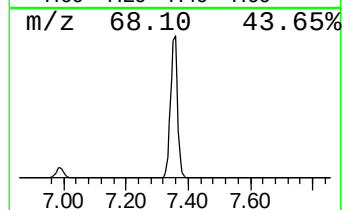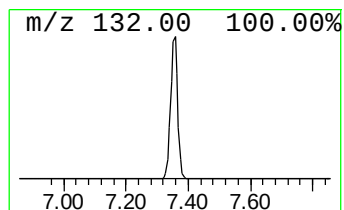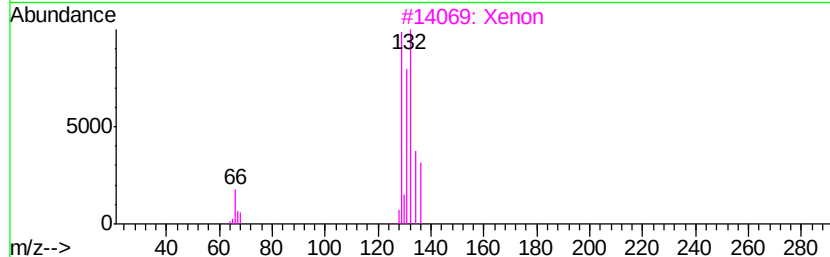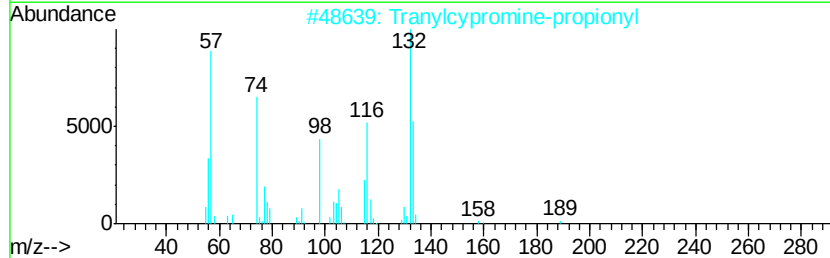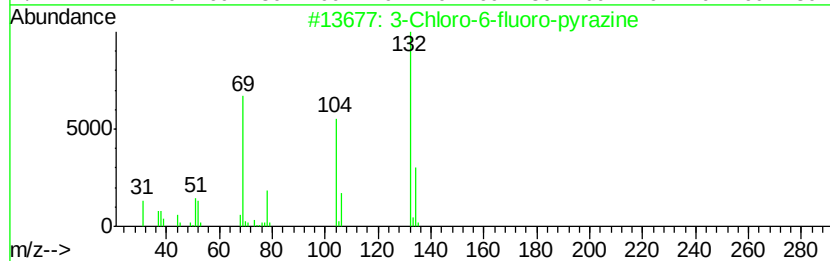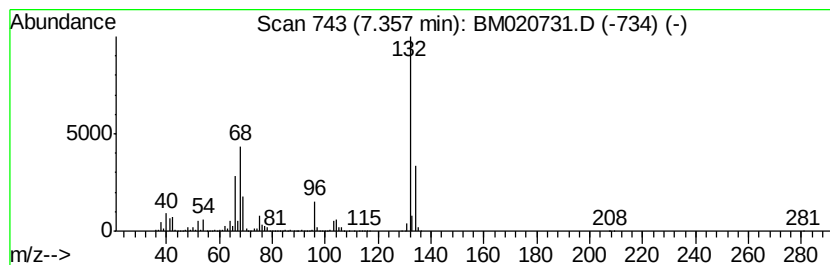

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060519\
Data File : BM020731.D
Acq On : 05 Jun 2019 11:54
Operator : HP/JU
Sample : PB191779BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119779BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.06	3.2	ng	298201	1	7.82	1871490	20.0
unknown7.36	7.36	98.4	ng	9209180	1	7.82	1871490	20.0