

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
 Data File : BM020743.D
 Acq On : 05 Jun 2019 19:10
 Operator : HP/JU
 Sample : PB120342BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120342BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	405	411	424	rBV	4971705	7014892	57.59%	8.940%
2	6.987	672	680	693	rBV	4781547	7601629	62.41%	9.687%
3	7.351	734	742	753	rBV	4876398	7754590	63.66%	9.882%
4	7.822	814	822	830	rVB	1068444	1680744	13.80%	2.142%
5	8.140	868	876	885	rBV	3757506	5961519	48.94%	7.597%
6	8.981	1010	1019	1032	rBV	2839030	4620012	37.93%	5.888%
7	10.610	1288	1296	1305	rBV	1333183	2201127	18.07%	2.805%
8	13.075	1708	1715	1729	rBV	7061152	10608865	87.09%	13.520%
9	14.457	1943	1950	1967	rBV2	1799736	2735592	22.46%	3.486%
10	15.945	2196	2203	2231	rBV	4637654	6710086	55.09%	8.551%
11	17.198	2410	2416	2429	rBV2	2033270	2989497	24.54%	3.810%
12	19.827	2857	2863	2872	rBV	10161873	12181095	100.00%	15.524%
13	21.380	3122	3127	3136	rBV	2422018	3144673	25.82%	4.008%
14	23.668	3509	3516	3526	rBV	1698228	3264257	26.80%	4.160%


Sum of corrected areas: 78468578

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
Data File : BM020743.D
Acq On : 05 Jun 2019 19:10
Operator : HP/JU
Sample : PB120342BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120342BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

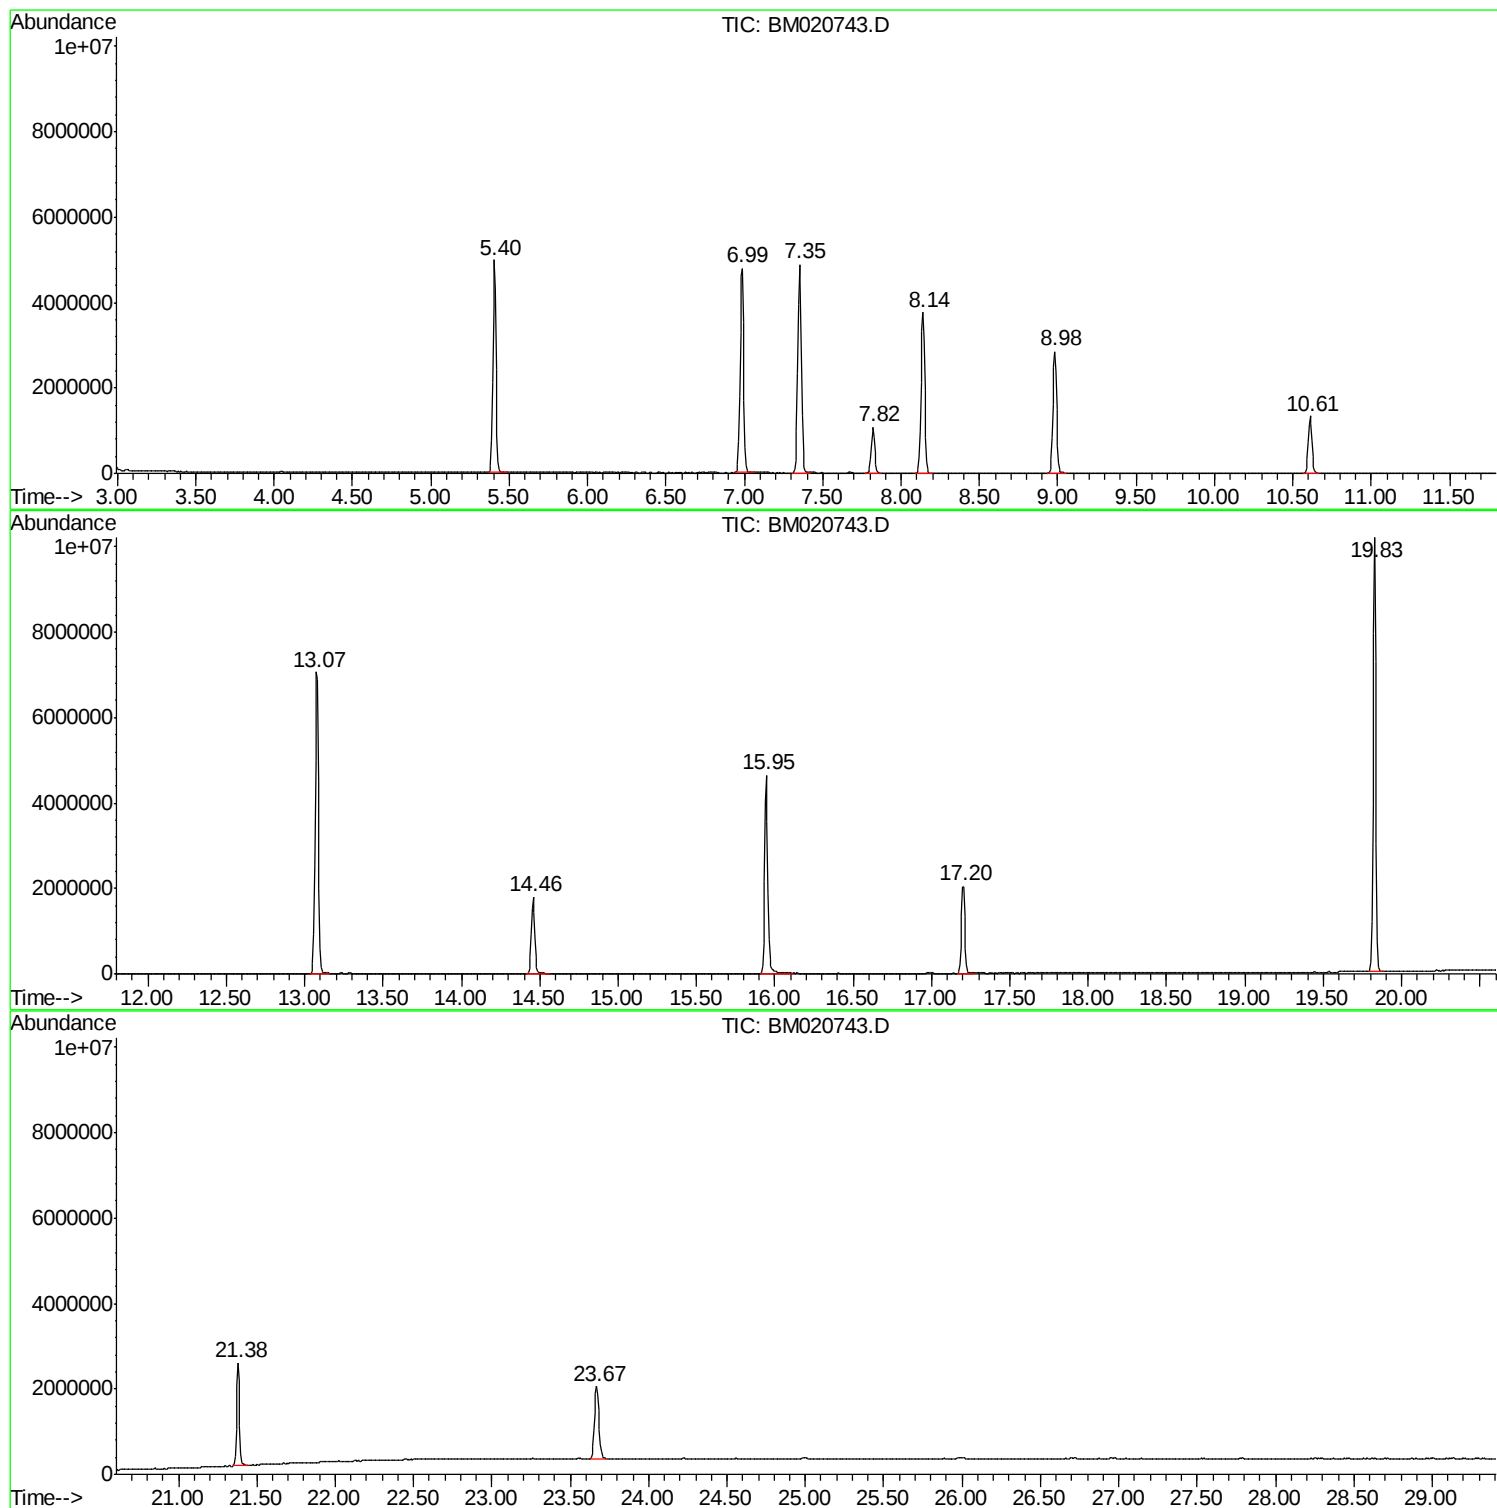

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
Data File : BM020743.D
Acq On : 05 Jun 2019 19:10
Operator : HP/JU
Sample : PB120342BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120342BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.35 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.35	92.28 ng	7754590	1,4-Dichlorobenzene-d4	7.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	10
4		Xenon	132	Xe	007440-63-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

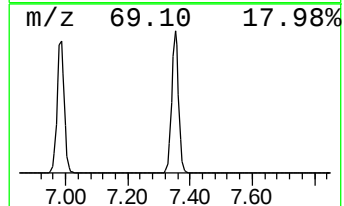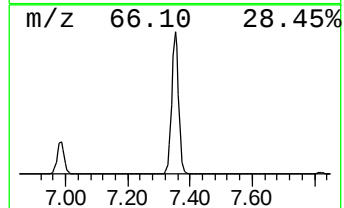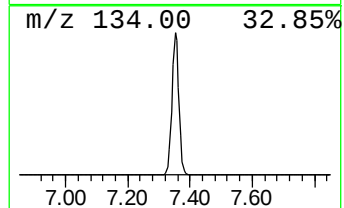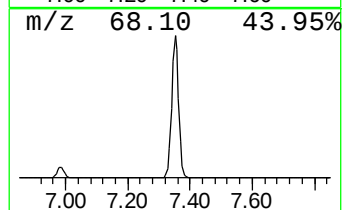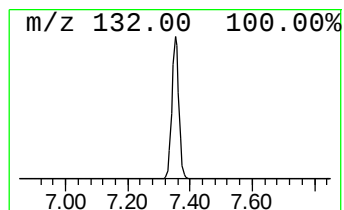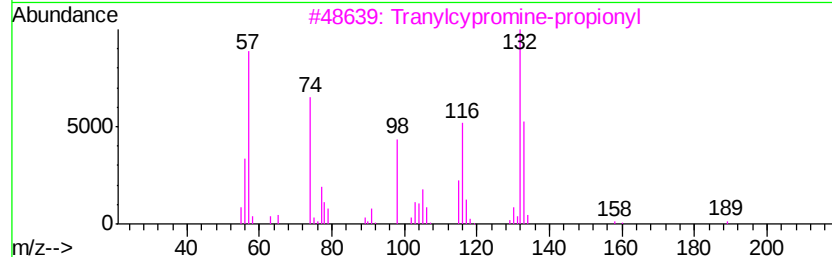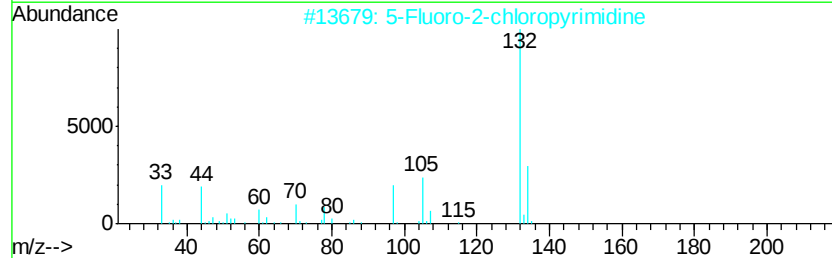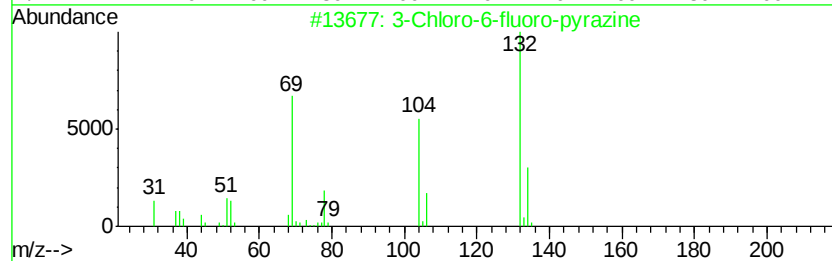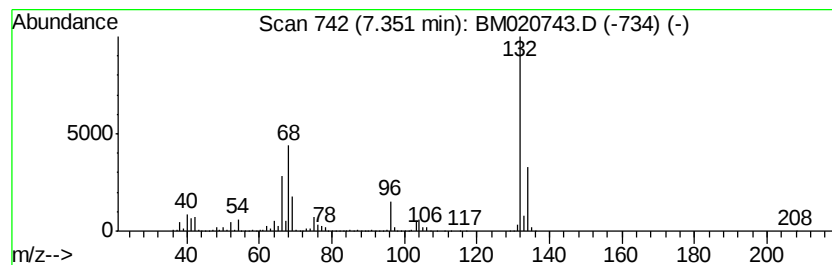

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060519\
Data File : BM020743.D
Acq On : 05 Jun 2019 19:10
Operator : HP/JU
Sample : PB120342BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120342BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.35	7.35	92.3	ng	7754590	1	7.82	1680740	20.0