


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060519\
Data File : BM020725.D
Acq On : 05 Jun 2019 08:13
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 31 15:48:49 2019

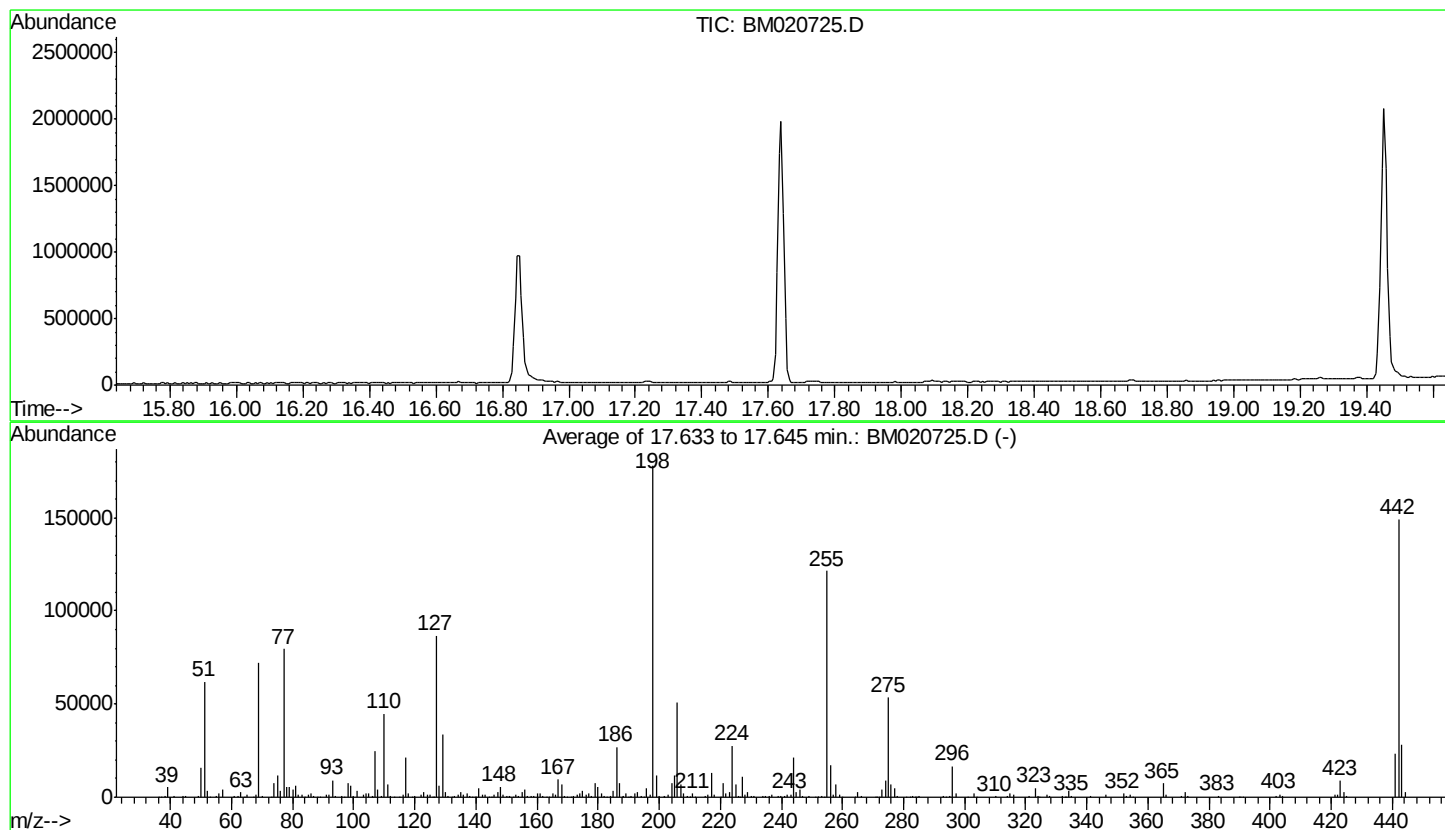

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	61897	PASS
68	69	0.00	2	2.0	1424	PASS
69	198	0.00	100	40.5	72074	PASS
70	69	0.00	2	0.6	467	PASS
127	198	10	80	48.8	86808	PASS
197	198	0.00	2	0.8	1406	PASS
198	198	100	100	100.0	177962	PASS
199	198	5	9	6.5	11554	PASS
275	198	10	60	30.1	53576	PASS
365	198	1	100	4.2	7543	PASS
441	198	0.01	100	13.1	23269	PASS
442	198	50	100	83.7	148928	PASS
443	442	15	24	19.0	28320	PASS