


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060519\
 Data File : BM020739.D
 Acq On : 05 Jun 2019 16:45
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 31 15:48:49 2019

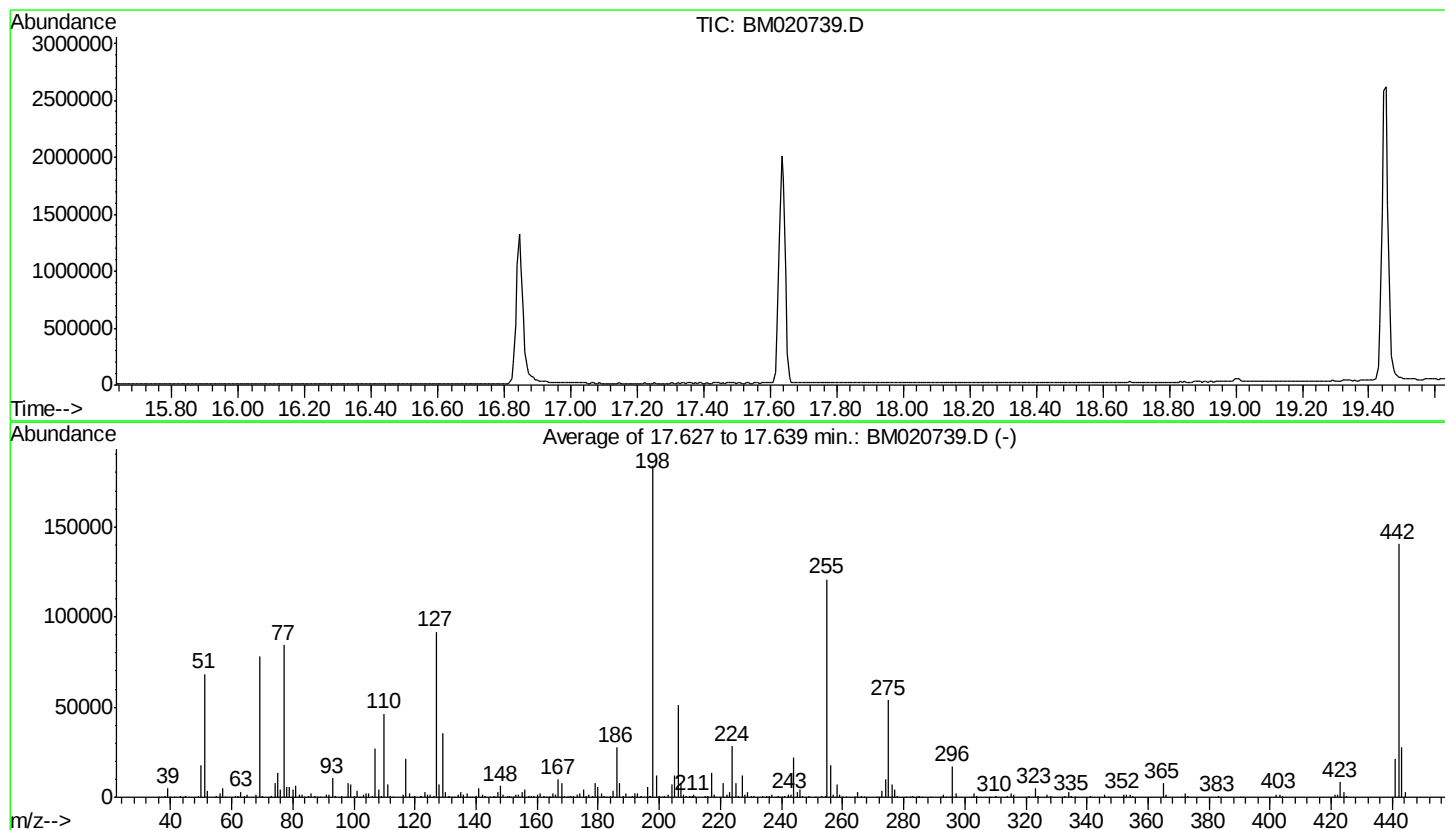

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	68477	PASS
68	69	0.00	2	1.8	1372	PASS
69	198	0.00	100	42.3	77808	PASS
70	69	0.00	2	0.6	481	PASS
127	198	10	80	49.8	91597	PASS
197	198	0.00	2	0.3	537	PASS
198	198	100	100	100.0	183914	PASS
199	198	5	9	6.7	12348	PASS
275	198	10	60	29.2	53706	PASS
365	198	1	100	4.1	7528	PASS
441	198	0.01	100	11.5	21181	PASS
442	198	50	100	76.3	140309	PASS
443	442	15	24	19.6	27436	PASS