


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
Data File : BM030992.D
Acq On : 16 Jul 2021 16:36
Operator : CG/JU
Sample : PB137665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK665

Manual Integrations
APPROVED

mohammad
7/19/2021 11:55:28 AM

Quant Time: Jul 16 17:08:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 16:49:56 2021
Response via : Initial Calibration

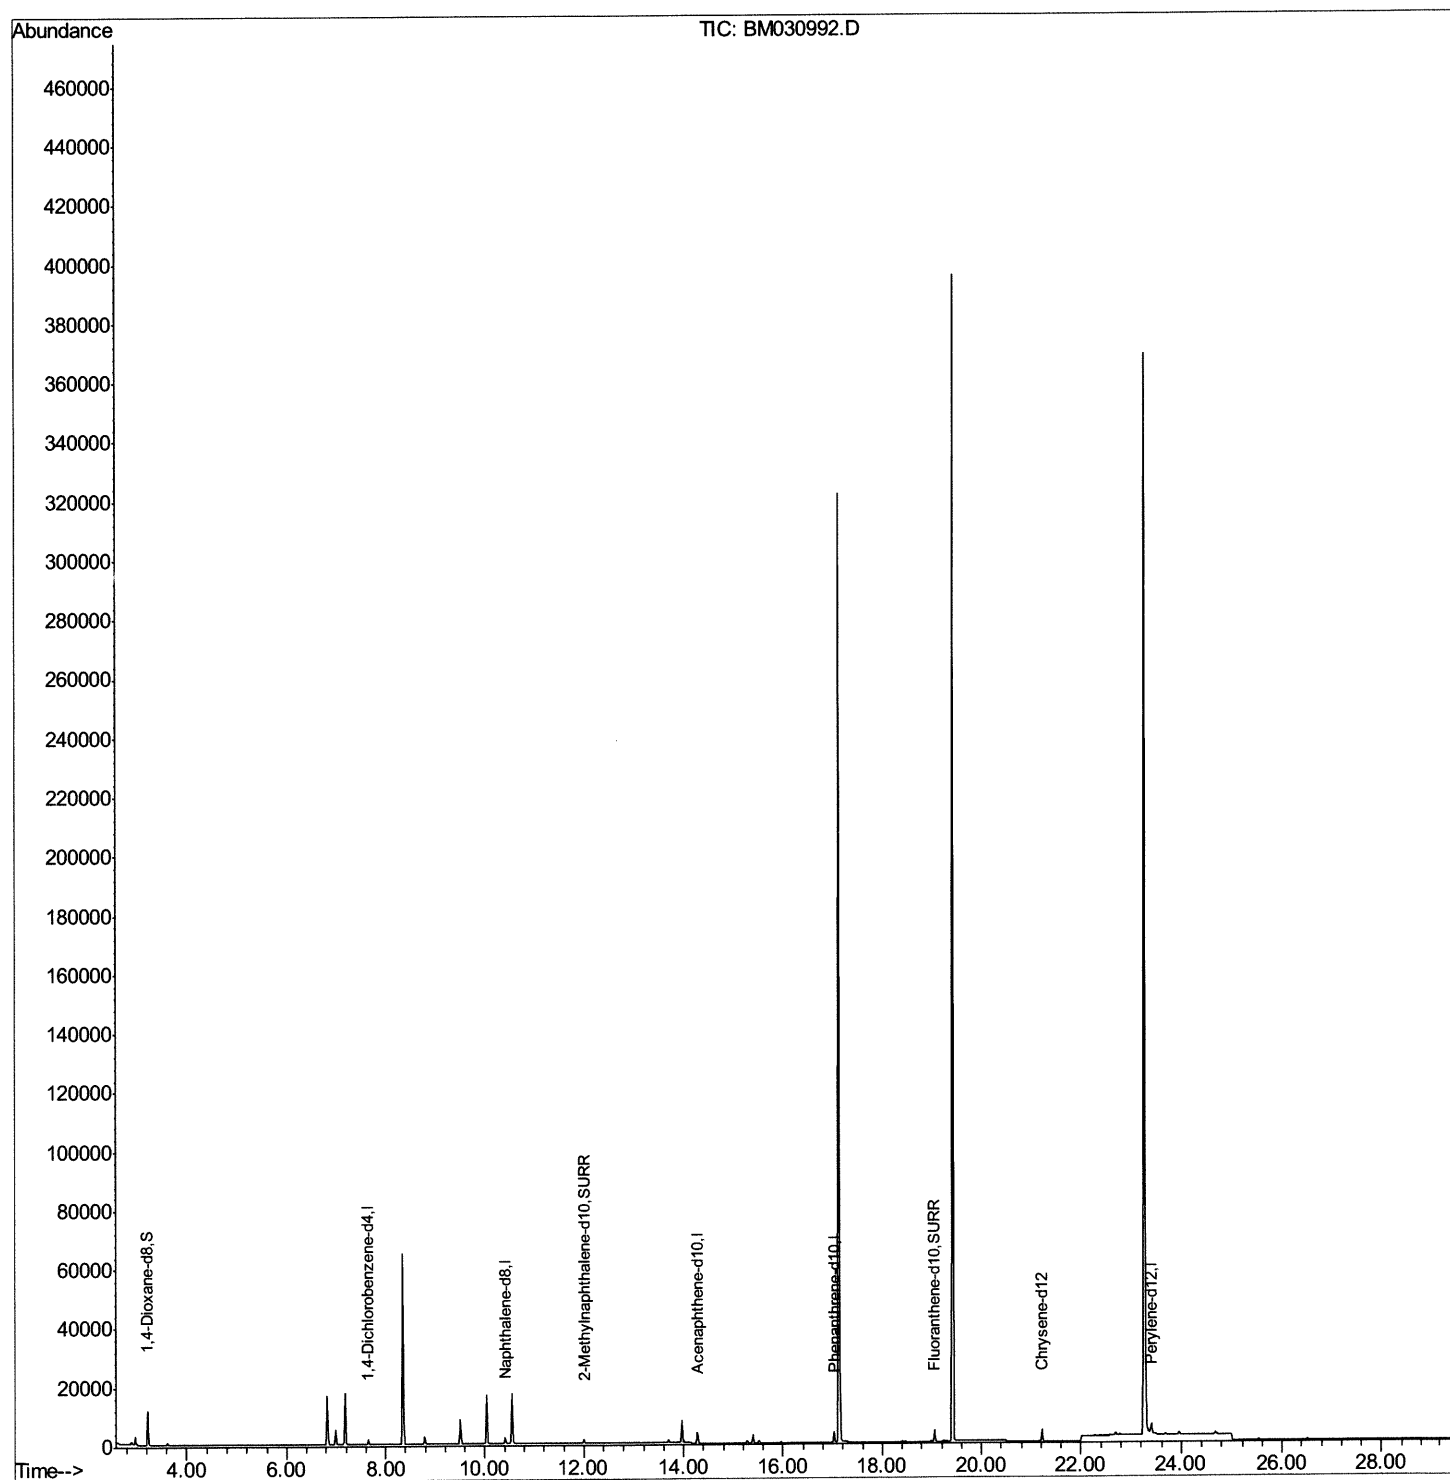

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
Data File : BM030992.D
Acq On : 16 Jul 2021 16:36
Operator : CG/JU
Sample : PB137665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK665

Manual Integrations
APPROVED

mohammad
7/19/2021 11:55:28 AM

Quant Time: Jul 16 17:06:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 16:49:56 2021
Response via : Initial Calibration

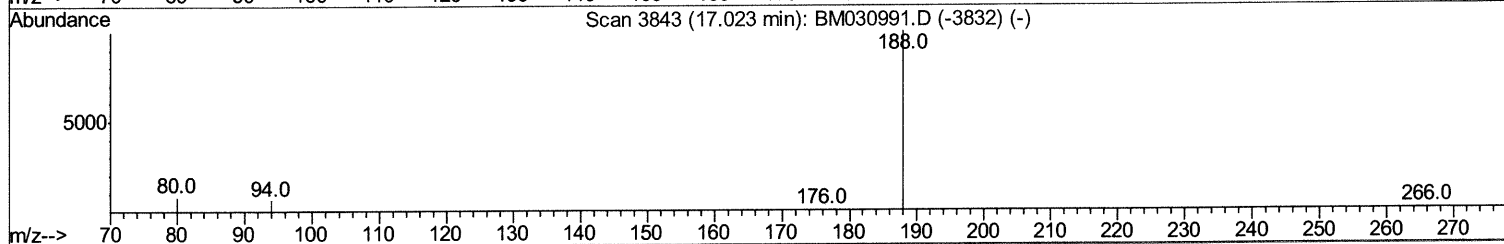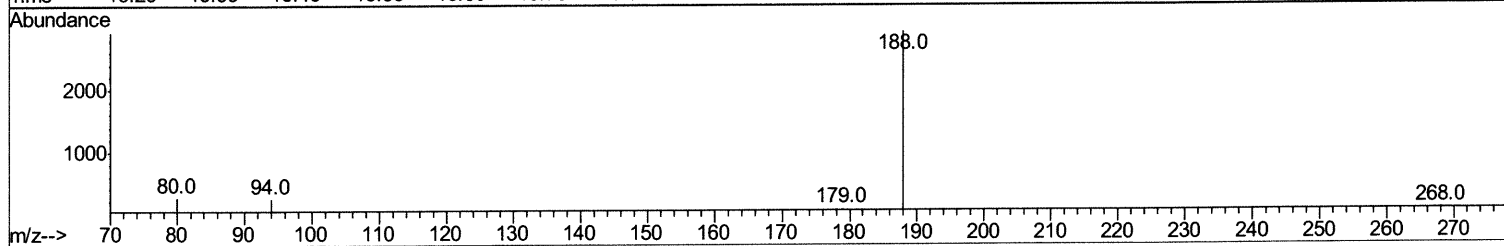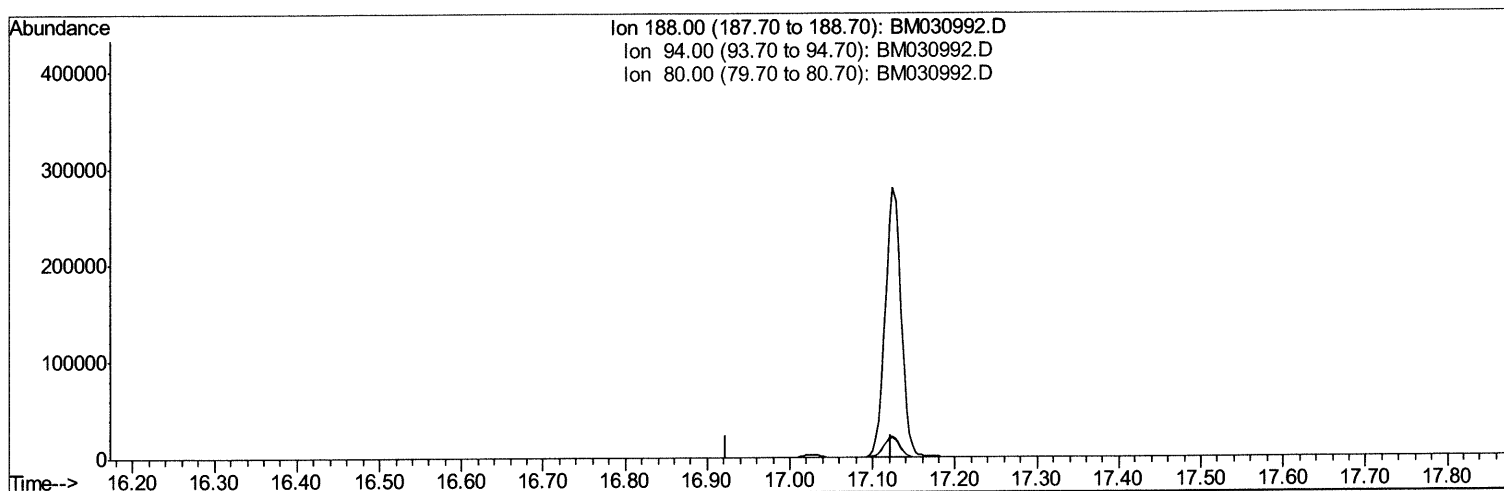

TIC: BM030992.D

(13) Phenanthrene-d10 (I)

17.023min (-17.023) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.70	0.00#
80.00	8.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030992.D
 Acq On : 16 Jul 2021 16:36
 Operator : CG/JU
 Sample : PB137665BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK665

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:55:28 AM

Quant Time: Jul 16 17:06:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 16:49:56 2021
 Response via : Initial Calibration

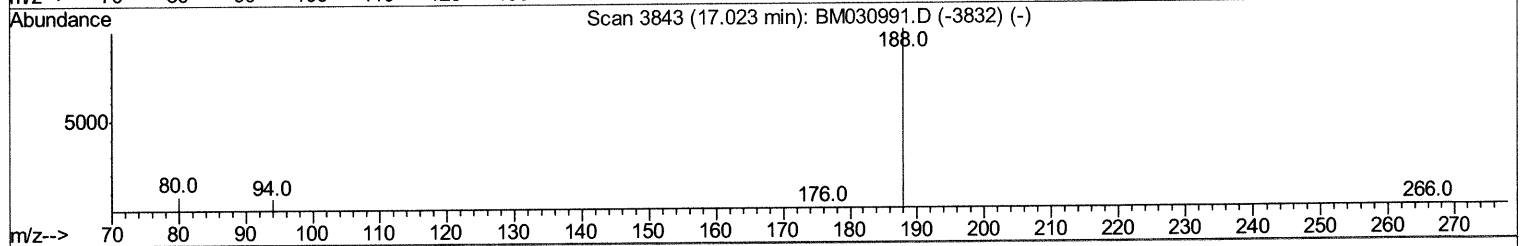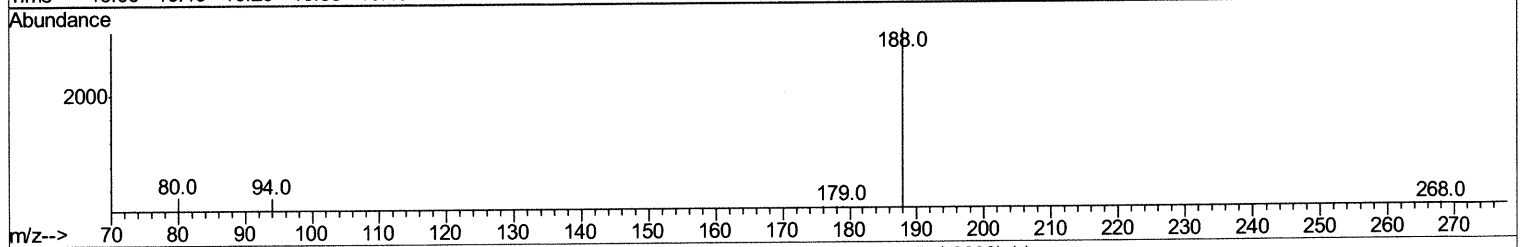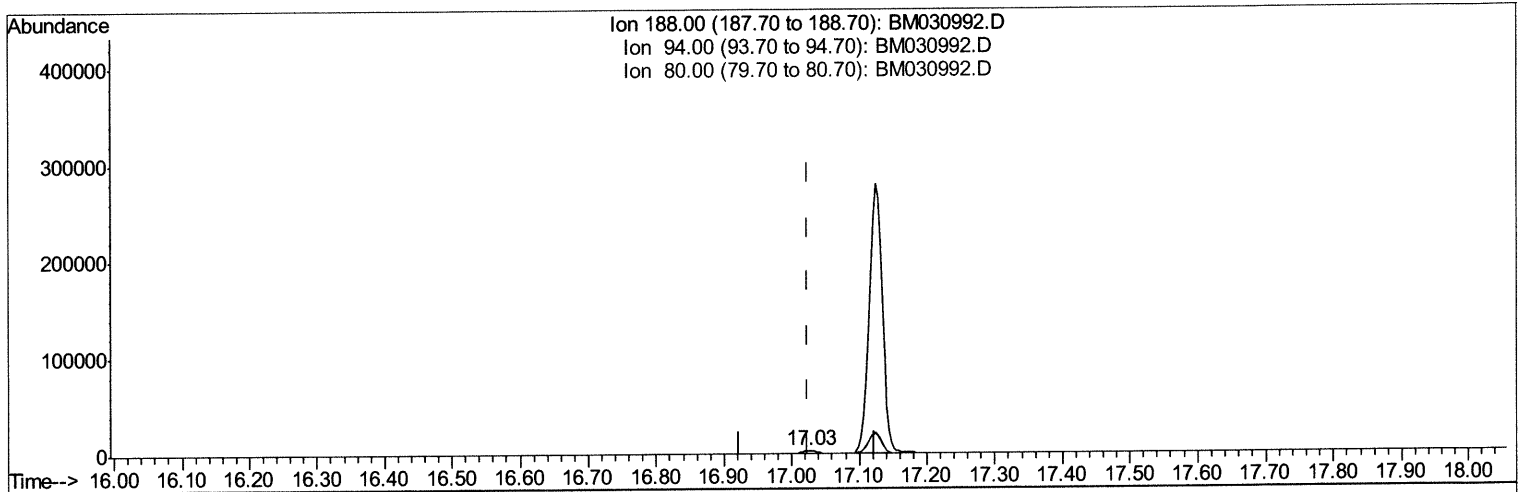

TIC: BM030992.D

(13) Phenanthrene-d10 (I)

17.027min (+0.003) 0.40ng/ul m 07/21/21 JU

response 4346

Ion	Exp%	Act%
188.00	100	100
94.00	8.70	8.25
80.00	8.50	8.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030992.D
 Acq On : 16 Jul 2021 16:36
 Operator : CG/JU
 Sample : PB137665BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK665

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:55:28 AM

Quant Time: Jul 16 17:08:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 16:49:56 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	853	0.40	ng/ul	0.00
4) Naphthalene-d8	10.41	136	2885	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.28	164	2043	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.03	188	4346m >	0.40	ng/ul >	0.00
17) Chrysene-d12	21.22	240	3724	0.40	ng/ul	0.00
23) Perylene-d12	23.40	264	4437	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	6426	7.33	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.01	152	1760	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.05	212	4520	0.36	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed