

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030994.D
 Acq On : 16 Jul 2021 17:51
 Operator : CG/JU
 Sample : PB137574BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK574

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:55:31 AM

Quant Time: Jul 16 18:24:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 16:49:56 2021
 Response via : Initial Calibration

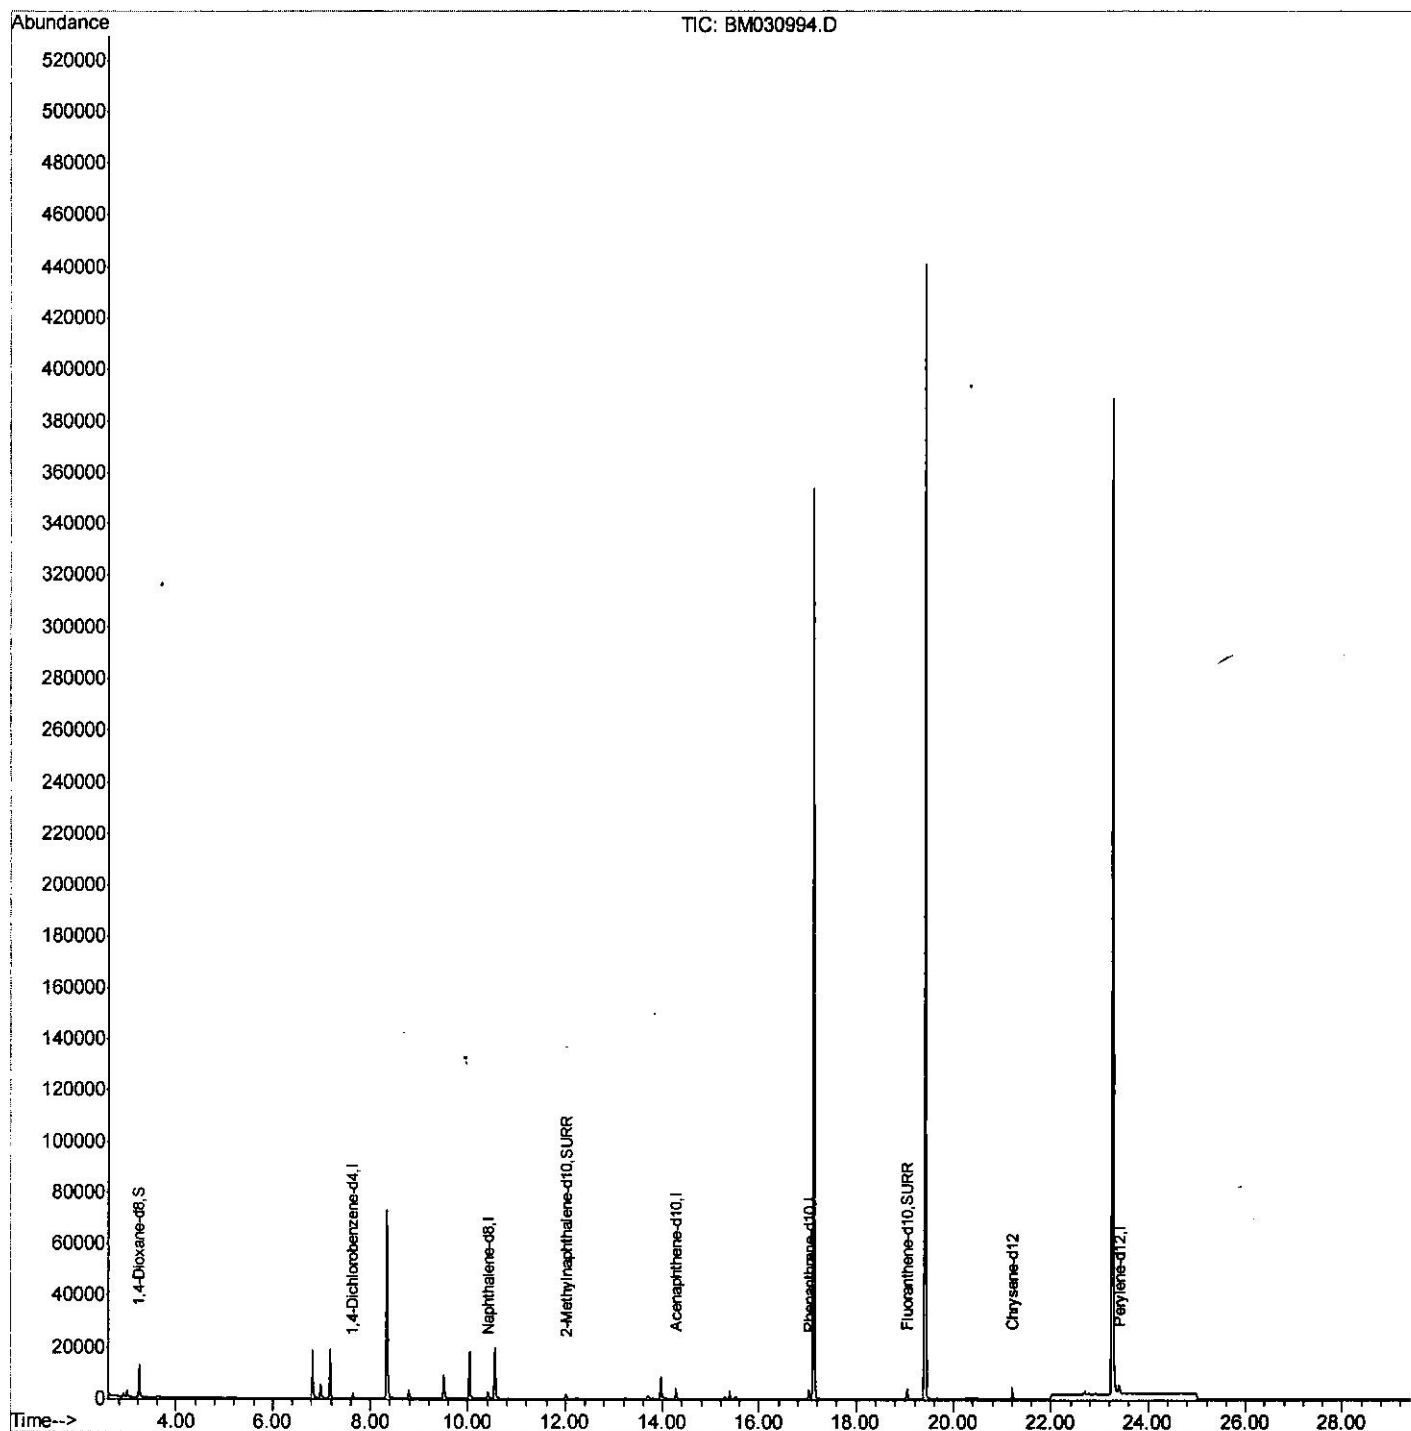

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030994.D
 Acq On : 16 Jul 2021 17:51
 Operator : CG/JU
 Sample : PB137574BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK574

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:55:31 AM

Quant Time: Jul 16 18:22:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 16:49:56 2021
 Response via : Initial Calibration

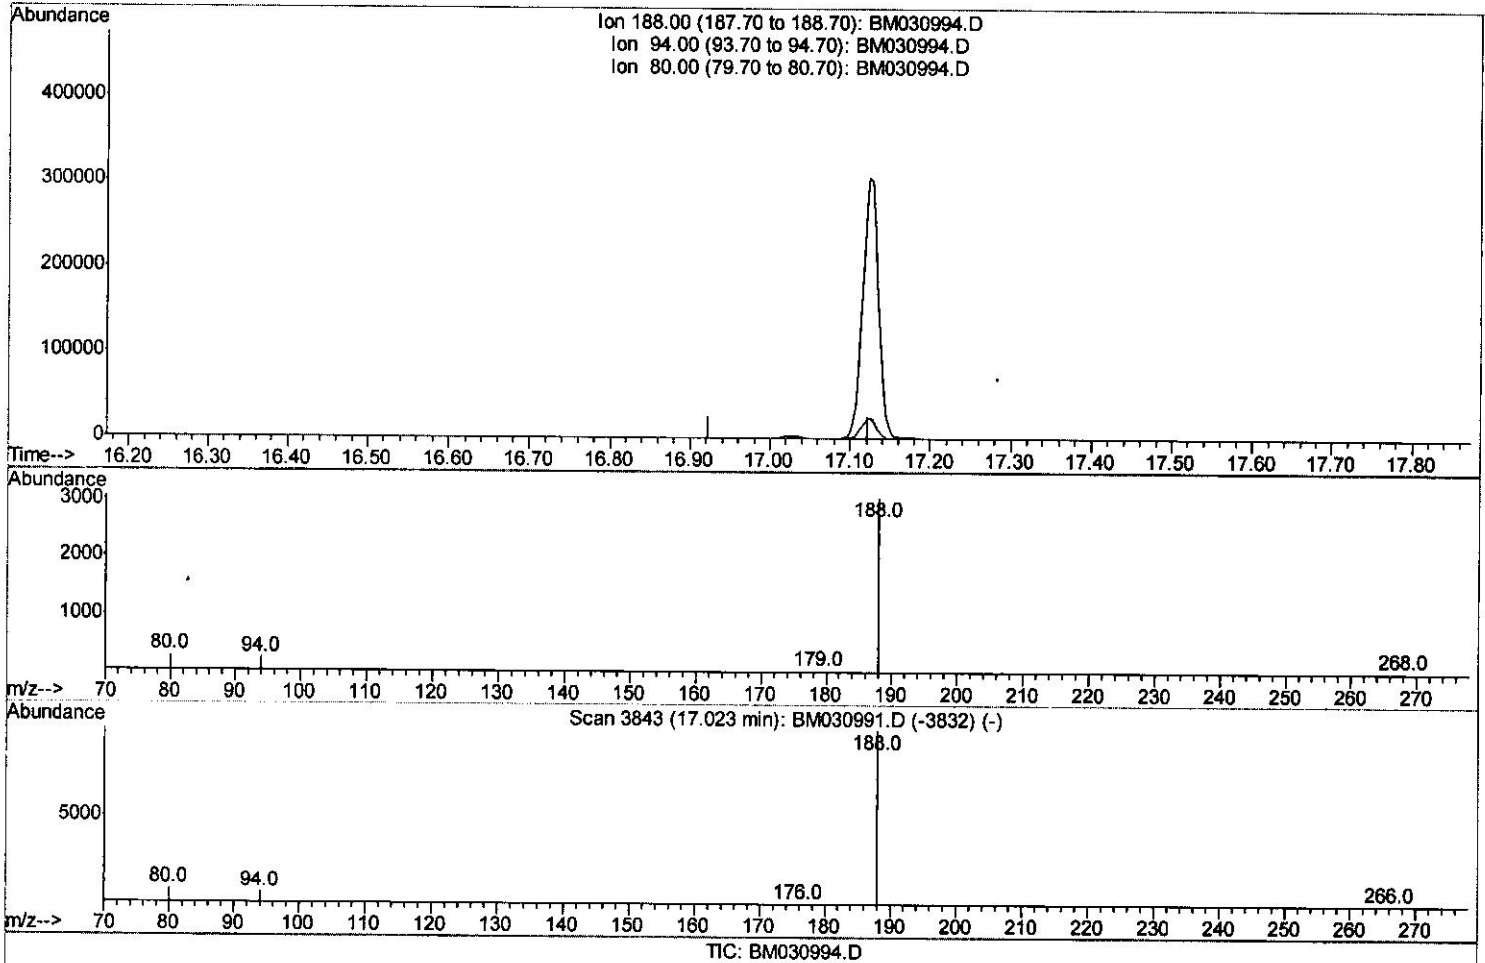

(13) Phenanthrene-d10 (I)
 17.023min (-17.023) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.70	0.00#
80.00	8.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030994.D
 Acq On : 16 Jul 2021 17:51
 Operator : CG/JU
 Sample : PB137574BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK574

Quant Time: Jul 16 18:22:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 16:49:56 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:55:31 AM

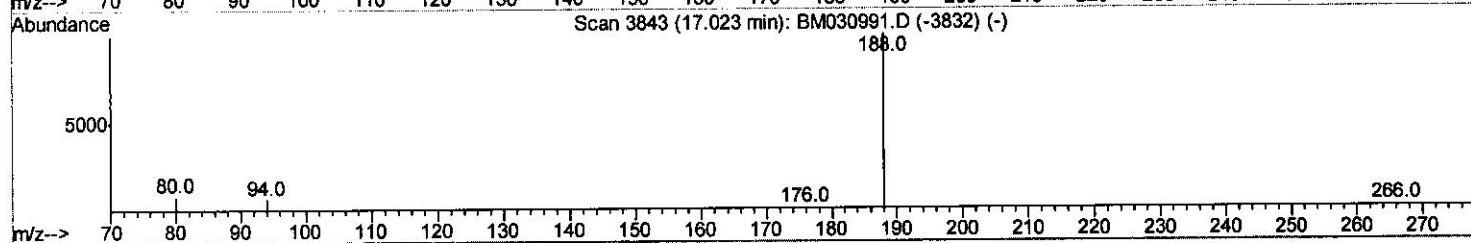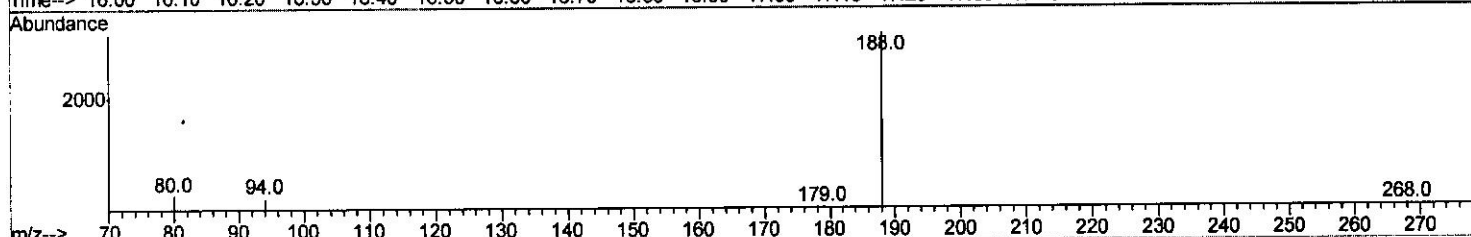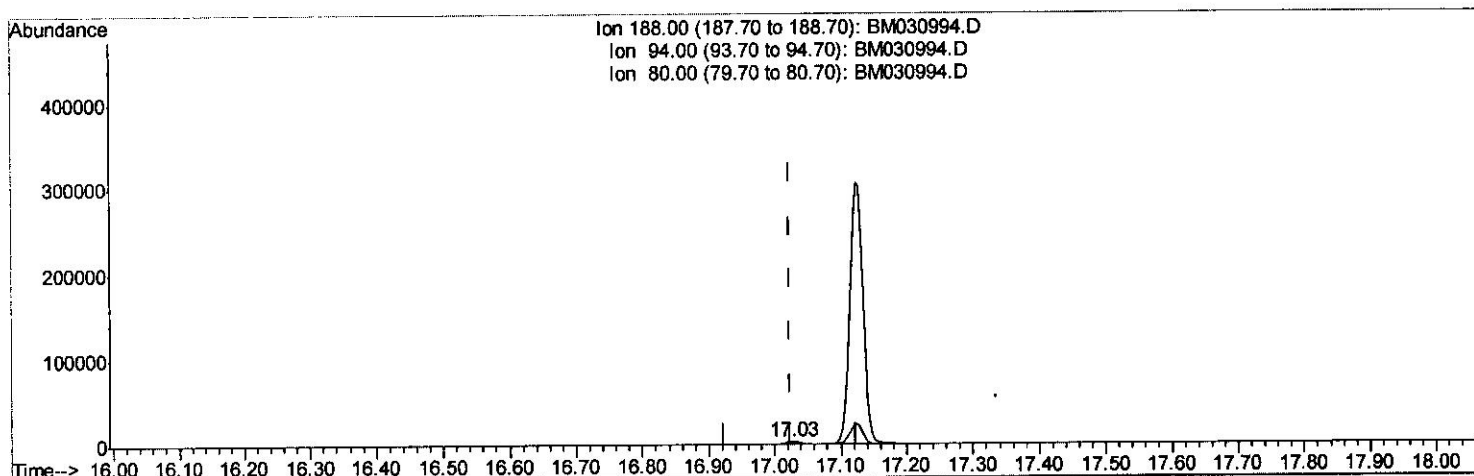

TIC: BM030994.D

(13) Phenanthrene-d10 (I)

17.027min (+0.004) 0.40ng/ul m JV: 7/19/21

response 4615

Ion	Exp%	Act%
188.00	100	100
94.00	8.70	7.90
80.00	8.50	9.54
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030994.D
 Acq On : 16 Jul 2021 17:51
 Operator : CG/JU
 Sample : PB137574BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK574

Quant Time: Jul 16 18:24:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 16:49:56 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:55:31 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	926	0.40	ng/ul	0.00
4) Naphthalene-d8	10.41	136	3083	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.28	164	2221	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.03	188	4615m	0.40	ng/ul	0.00
17) Chrysene-d12	21.21	240	3967	0.40	ng/ul	0.00
23) Perylene-d12	23.40	264	4570	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	7094	7.45	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.01	152	2022	0.38	ng/ul	0.00
18) Fluoranthene-d10	19.05	212	4935	0.37	ng/ul	0.00

SV 07/19/21

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed