
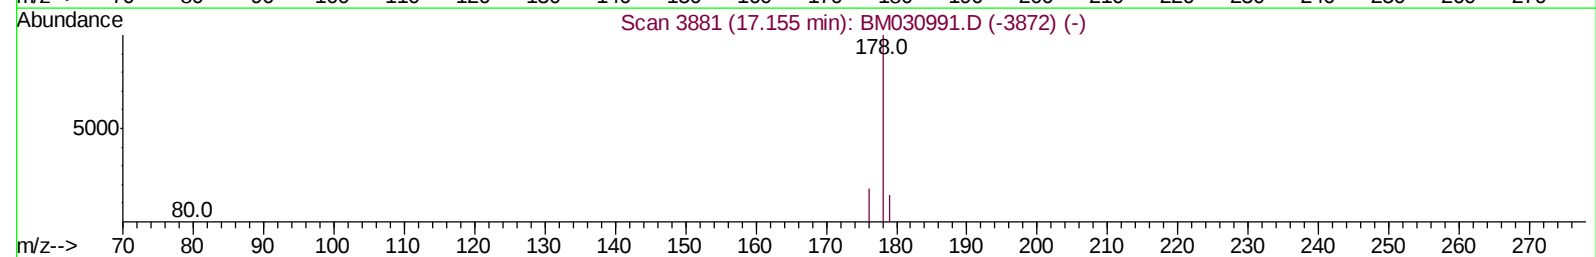
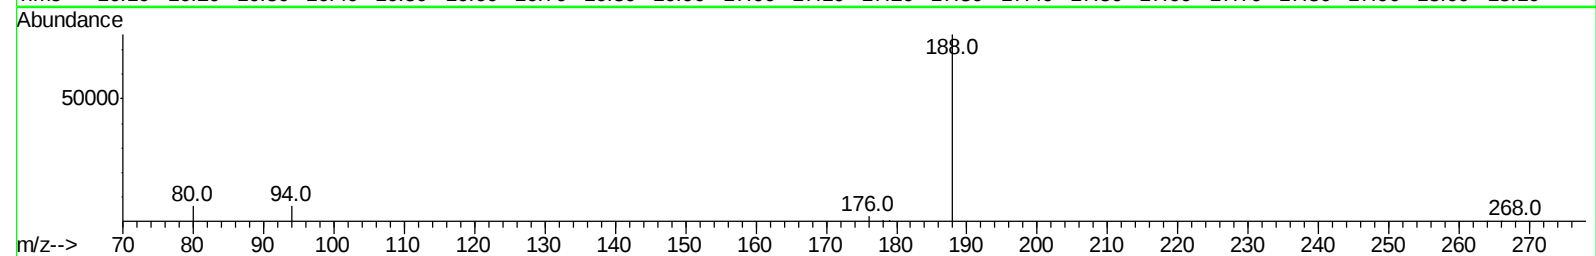


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
Data File : BM030997.D
Acq On : 16 Jul 2021 19:43
Operator : CG/JU
Sample : M2905-21DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 16 23:26:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 16:49:56 2021
Response via : Initial Calibration

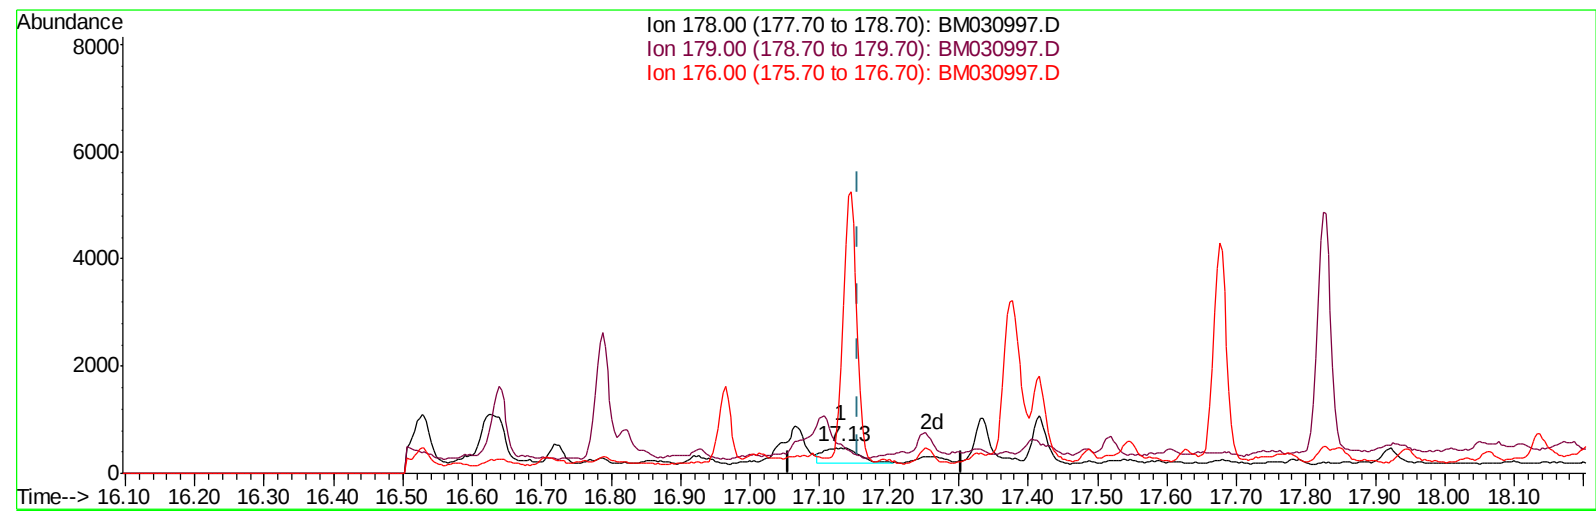

TIC: BM030997.D

(16) Anthracene

17.131min (-0.024) 0.04ng/ul

response 933

Ion	Exp%	Act%
178.00	100	100
179.00	18.10	111.39#
176.00	20.10	410.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
 Data File : BM030997.D
 Acq On : 16 Jul 2021 19:43
 Operator : CG/JU
 Sample : M2905-21DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 16 23:30:44 2021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jul 16 16:49:56 2021

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	1198	0.40	ng/ul	0.00
4) Naphthalene-d8	10.41	136	4585	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.28	164	4803	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.03	188	7576	0.40	ng/ul	0.00
17) Chrysene-d12	21.21	240	6339	0.40	ng/ul	0.00
23) Perylene-d12	23.40	264	5922	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	671	0.54	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.01	152	770	0.10	ng/ul	0.00
18) Fluoranthene-d10	19.05	212	2029	0.10	ng/ul	0.00
Target Compounds				Ovalue		
2) 1,4-Dioxane	3.26	88	270	0.196	ng/ul#	81
5) Naphthalene	10.46	128	33887	2.477	ng/ul	95
7) 2-Methylnaphthalene	12.08	142	15100	1.562	ng/ul	98
8) 1-Methylnaphthalene	12.30	142	10610	1.123	ng/ul	96
11) Acenaphthene	14.34	153	708	0.042	ng/ul#	84
12) Fluorene	15.33	166	1700	0.084	ng/ul#	94
14) Pentachlorophenol	16.68	266	65	0.024	ng/ul	93
15) Phenanthrene	17.06	178	1619	0.068	ng/ul#	30
19) Fluoranthene	19.06	202	652	0.023	ng/ul#	8

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071621\
Data File : BM030997.D
Acq On : 16 Jul 2021 19:43
Operator : CG/JU
Sample : M2905-21DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 16 23:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 16:49:56 2021
Response via : Initial Calibration

