
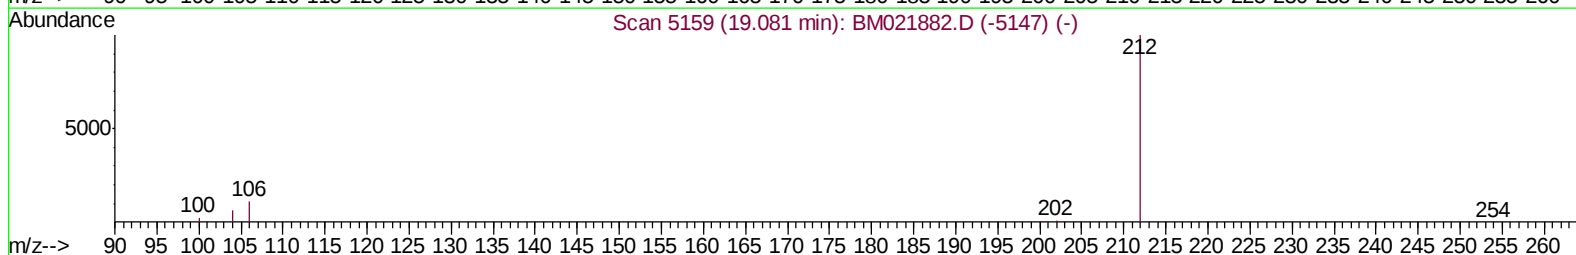
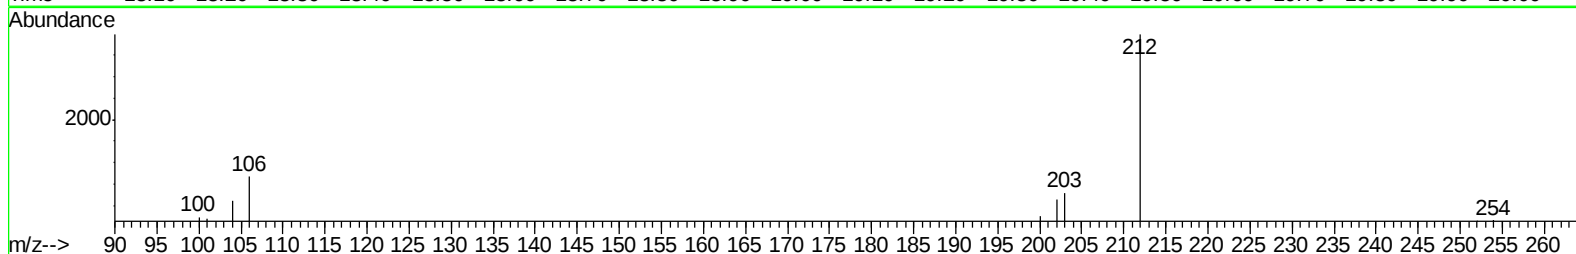


Data File : BM021883.D  
Acq On : 07 Aug 2019 06:50  
Operator : HP/JU  
Sample : K3893-11  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Aug 07 08:31:50 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 07 08:28:11 2019  
Response via : Initial Calibration

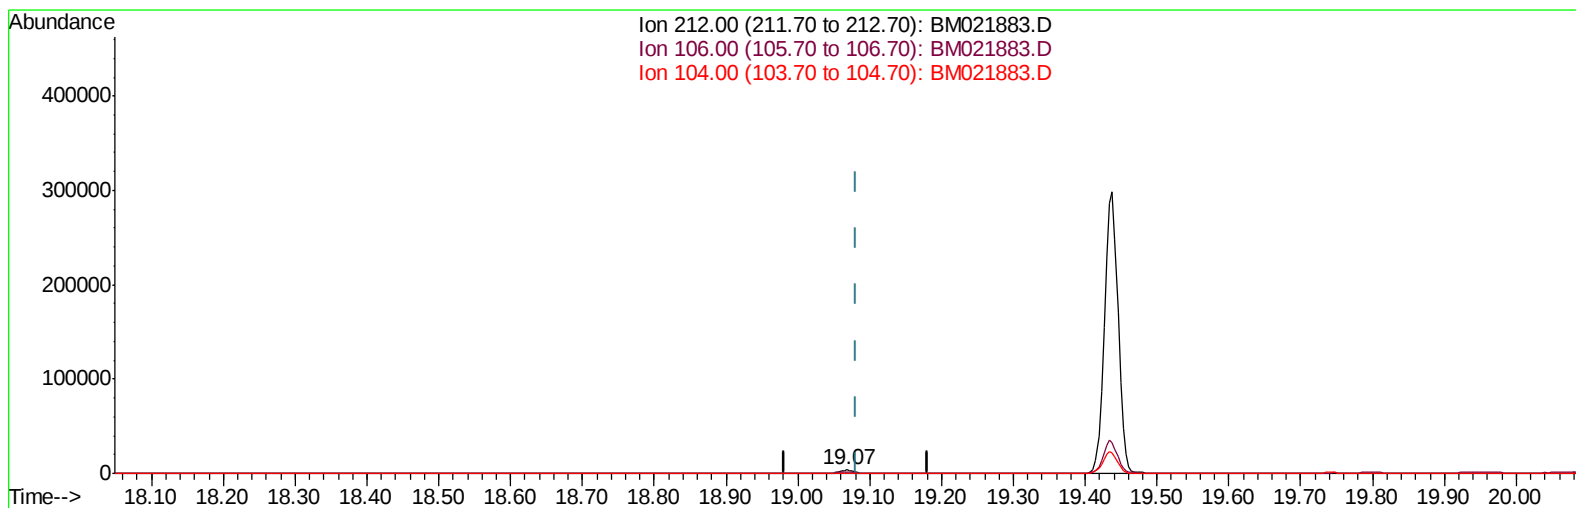

TIC: BM021883.D

(14) Fluoranthene-d10 (SURR)

19.068min (-0.013) 0.30ng/ul m

response 4636

| Ion    | Exp% | Act%  |
|--------|------|-------|
| 212.00 | 100  | 100   |
| 106.00 | 9.90 | 0.00# |
| 104.00 | 6.00 | 0.00# |
| 0.00   | 0.00 | 0.00  |