
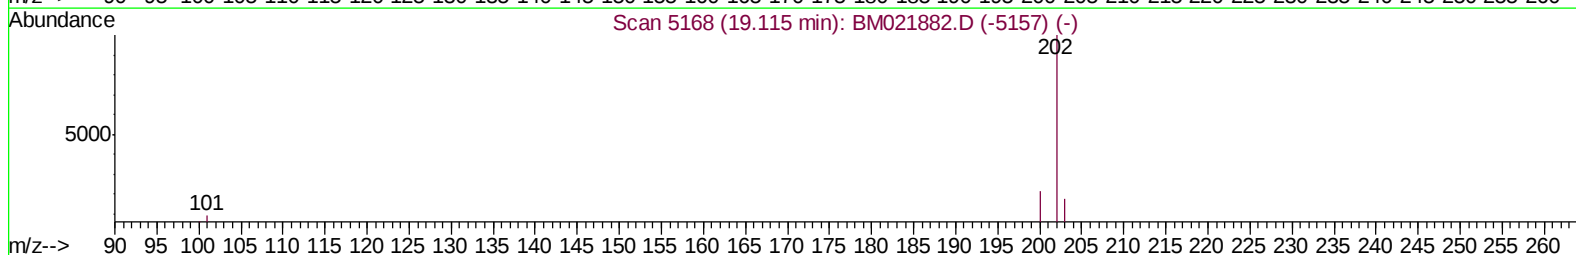
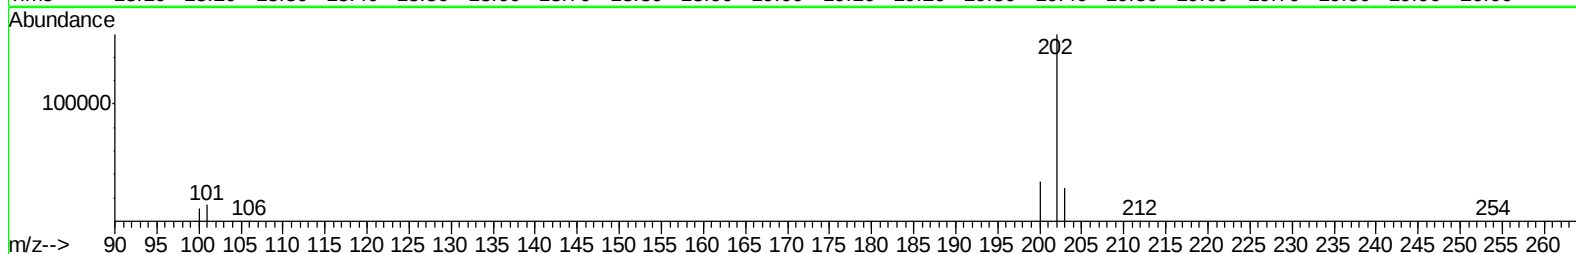


Data File : BM021883.D
Acq On : 07 Aug 2019 06:50
Operator : HP/JU
Sample : K3893-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Aug 07 08:31:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

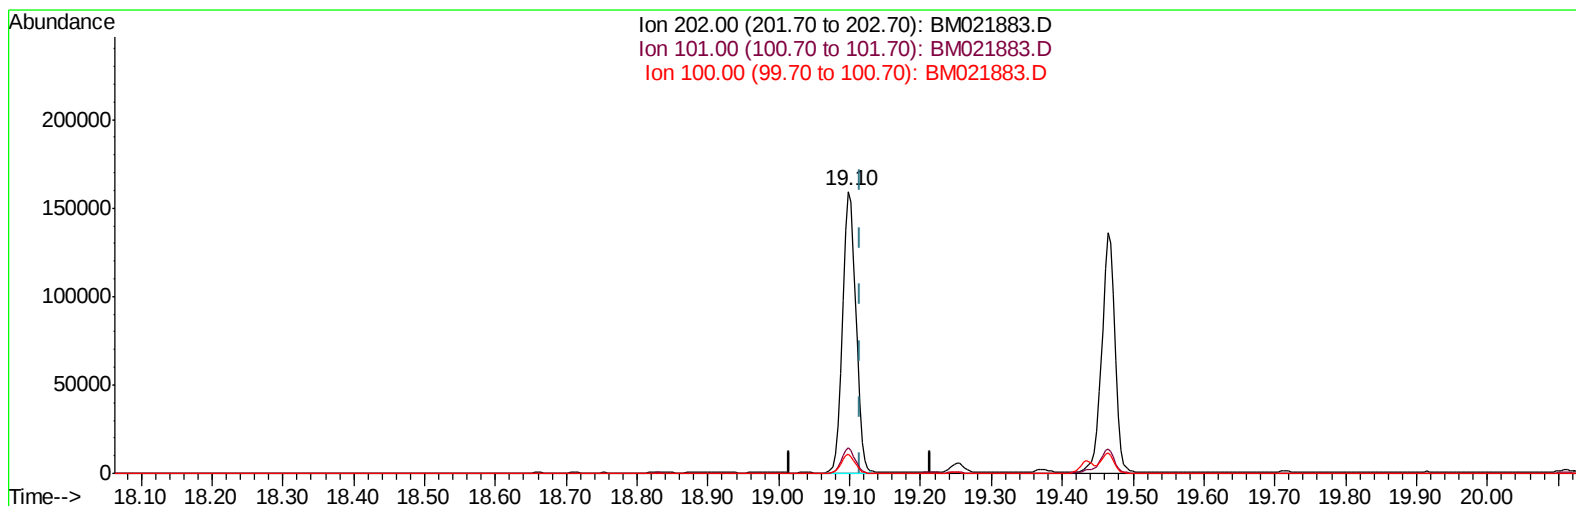

TIC: BM021883.D

(15) Fluoranthene (C)

19.098min (-0.017) 11.61ng/ul m

response 209084

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	8.92
100.00	8.10	6.97
0.00	0.00	0.00