
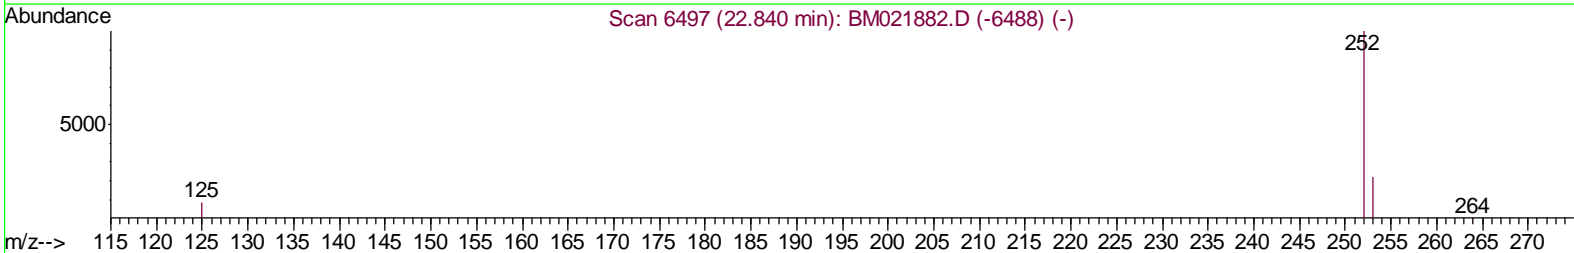
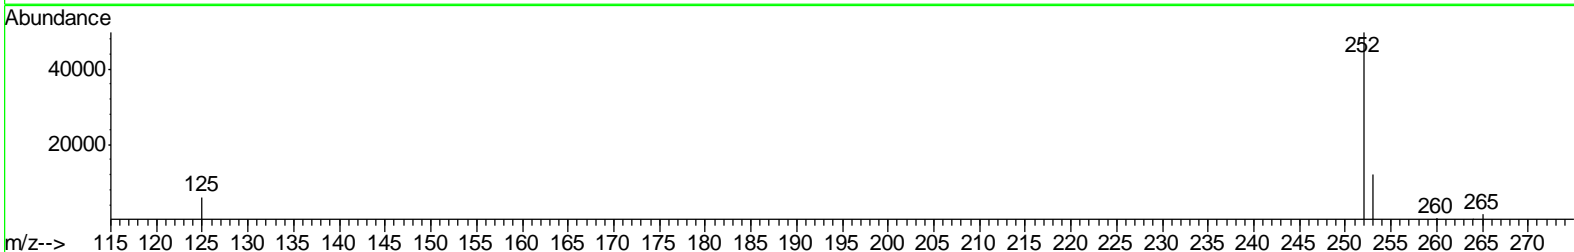


Data File : BM021883.D
Acq On : 07 Aug 2019 06:50
Operator : HP/JU
Sample : K3893-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Aug 07 08:34:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

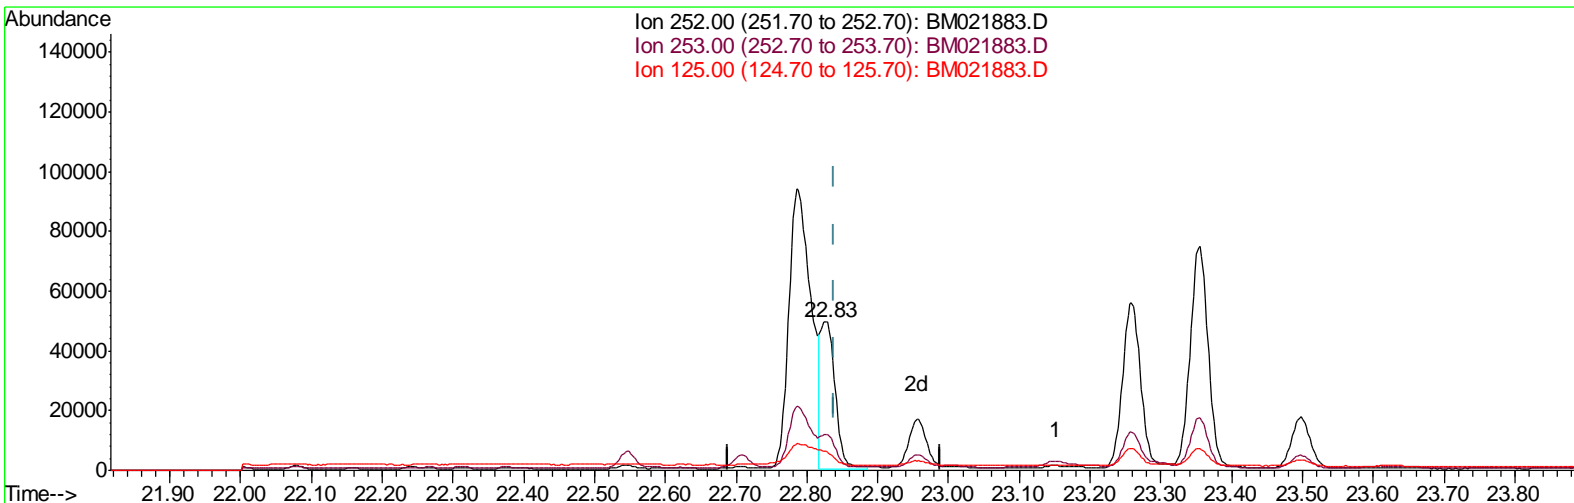

TIC: BM021883.D

(22) Benzo(k)fluoranthene
22.829min (-0.010) 3.46ng/ul m
response 70201

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.34#
125.00	15.20	12.09#
0.00	0.00	0.00