
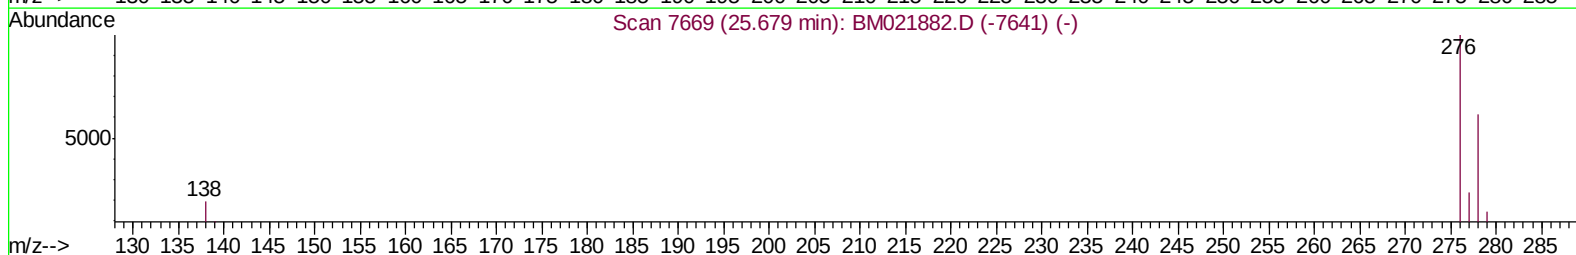
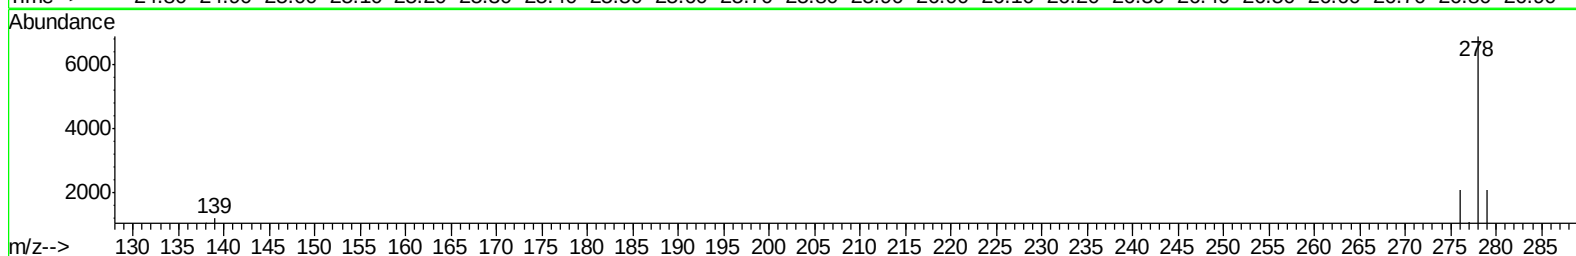


Data File : BM021883.D
Acq On : 07 Aug 2019 06:50
Operator : HP/JU
Sample : K3893-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Aug 07 08:34:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

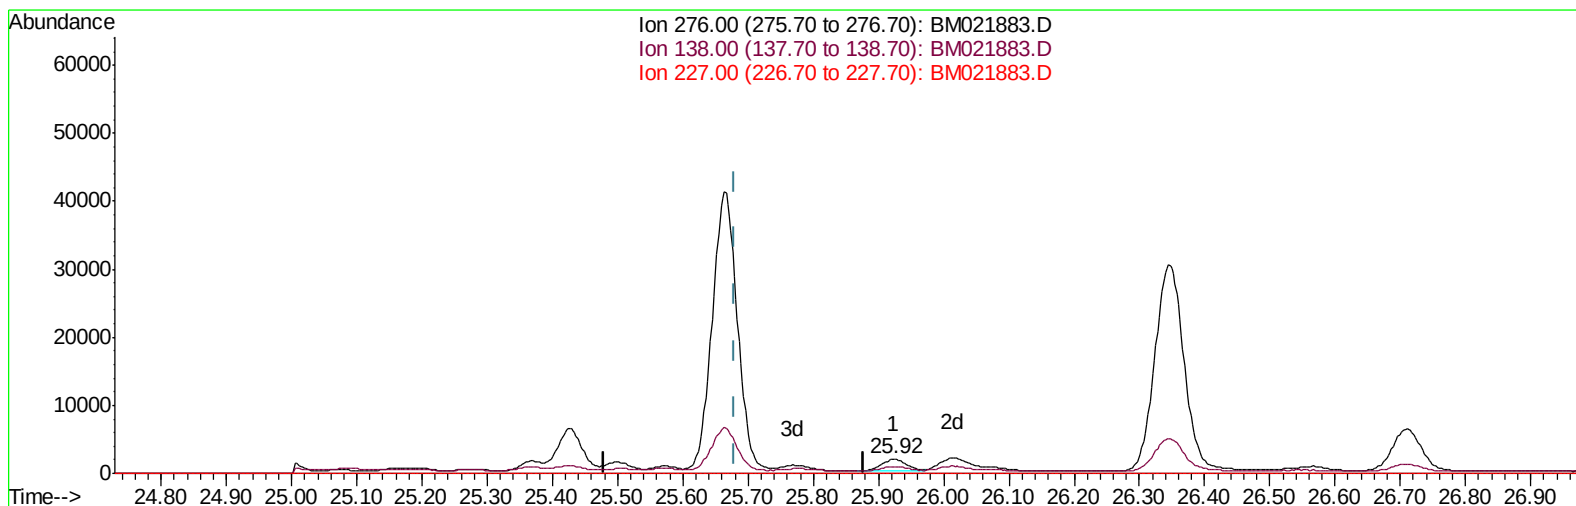

TIC: BM021883.D

(24) Indeno(1,2,3-cd)pyrene

25.923min (+0.244) 0.21ng/ul

response 4648

Ion	Exp%	Act%
276.00	100	100
138.00	18.90	43.33#
227.00	0.00	0.00
0.00	0.00	0.00