
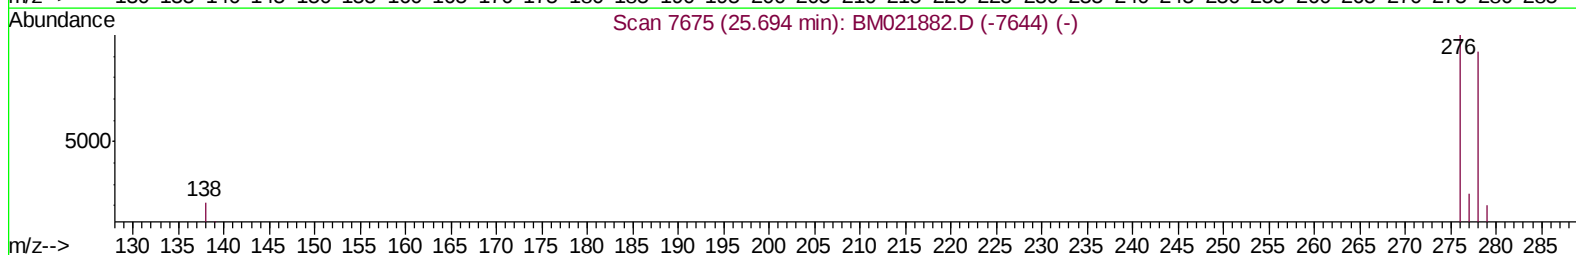
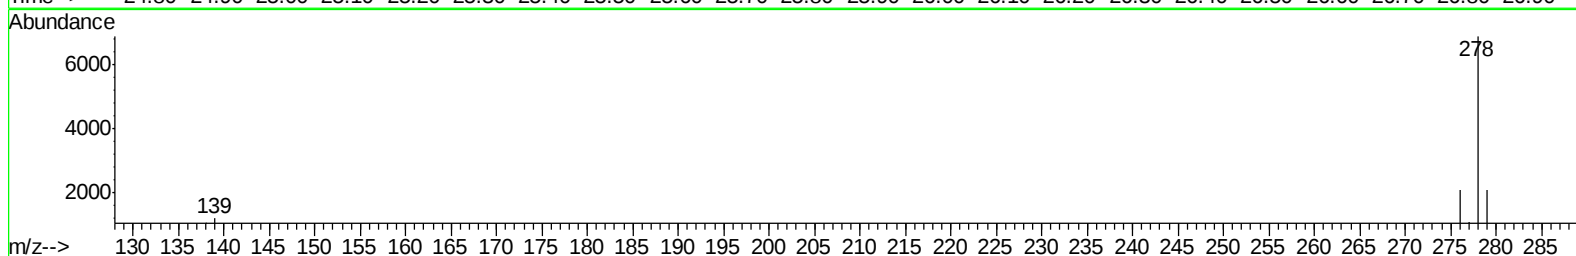


Data File : BM021883.D  
Acq On : 07 Aug 2019 06:50  
Operator : HP/JU  
Sample : K3893-11  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Aug 07 08:34:22 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 07 08:28:11 2019  
Response via : Initial Calibration

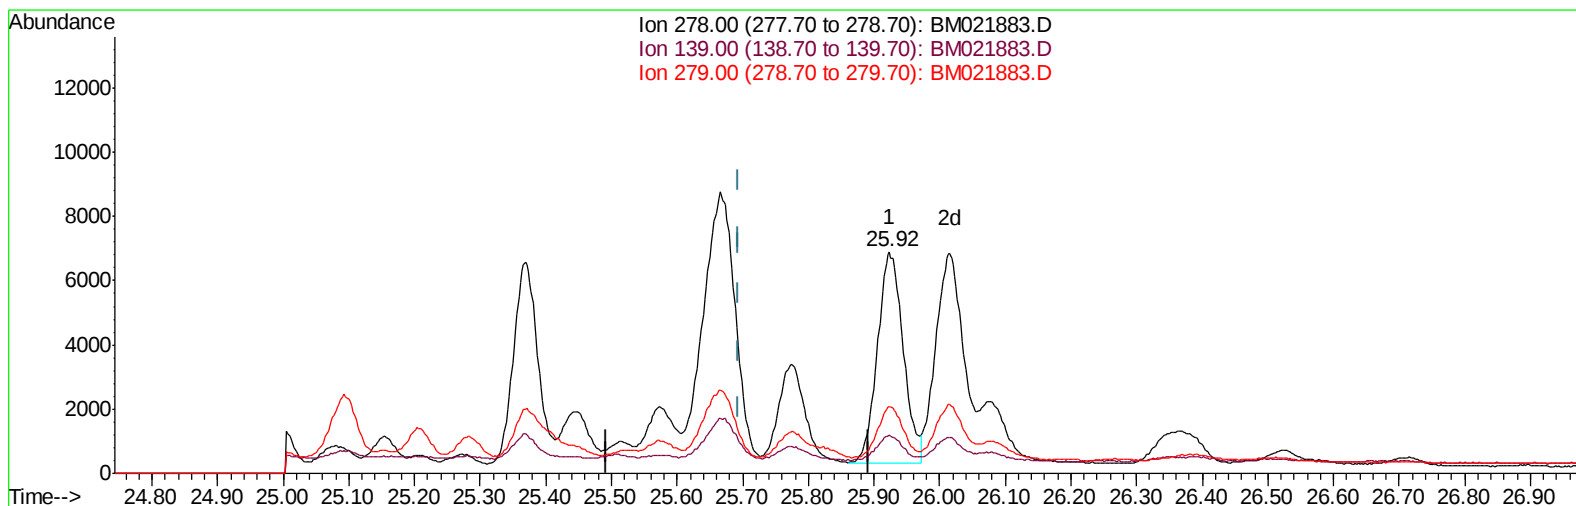

TIC: BM021883.D

(25) Dibenzo(a,h)anthracene

25.923min (+0.230) 1.01ng/ul

response 17745

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 278.00 | 100   | 100   |
| 139.00 | 17.70 | 17.14 |
| 279.00 | 35.40 | 30.11 |
| 0.00   | 0.00  | 0.00  |