
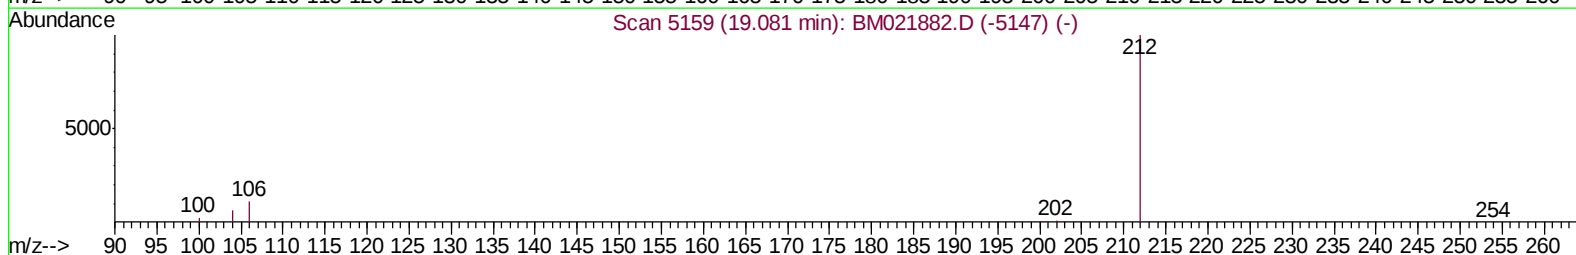
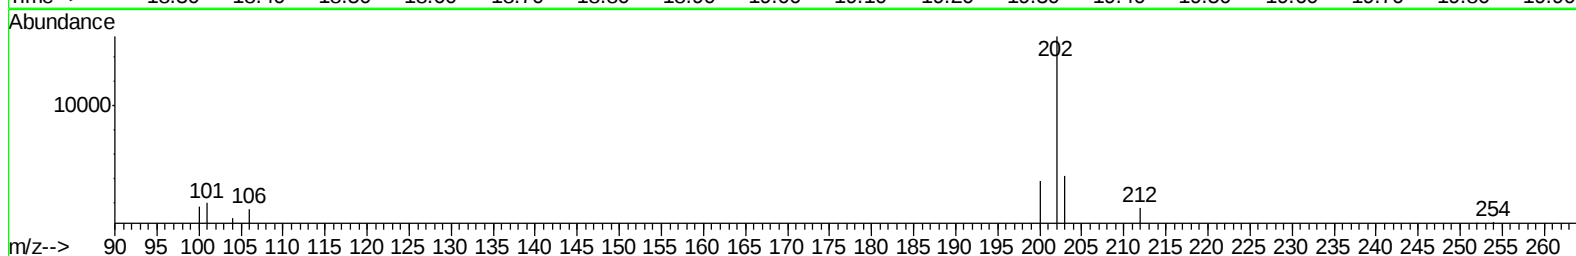


Data File : BM021884.D
Acq On : 07 Aug 2019 07:26
Operator : HP/JU
Sample : K3893-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Aug 07 08:49:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

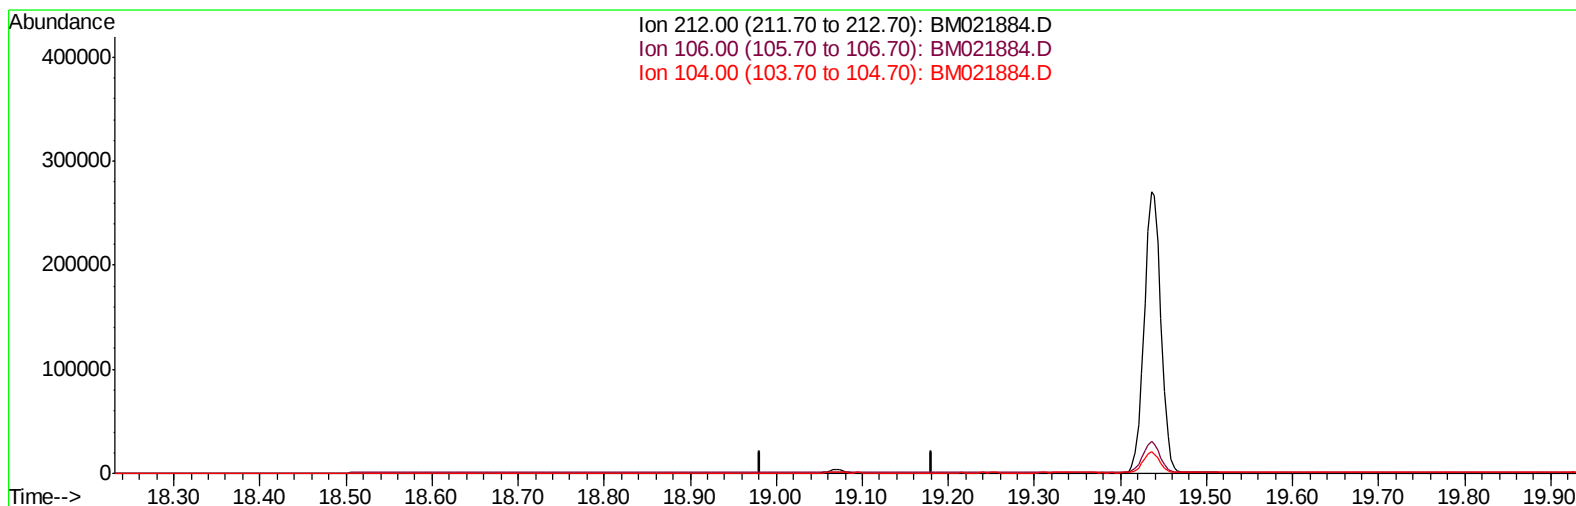

TIC: BM021884.D

(14) Fluoranthene-d10 (SURRE)

19.081min (-19.081) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00