
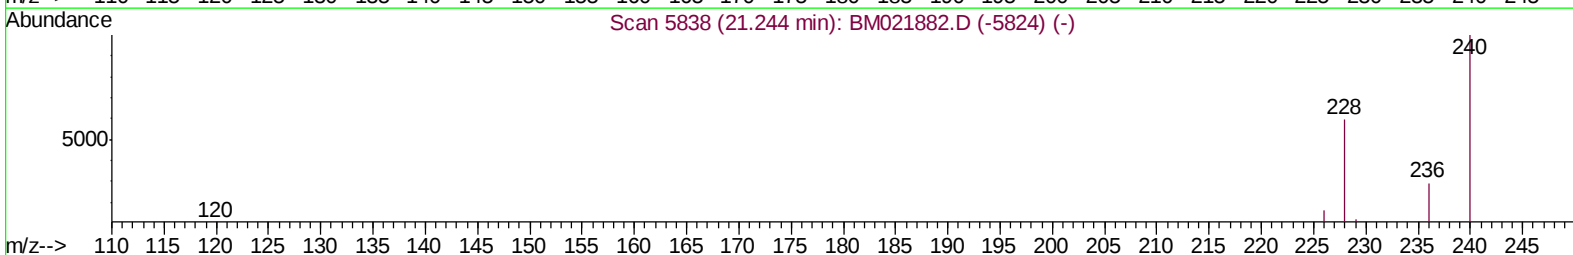
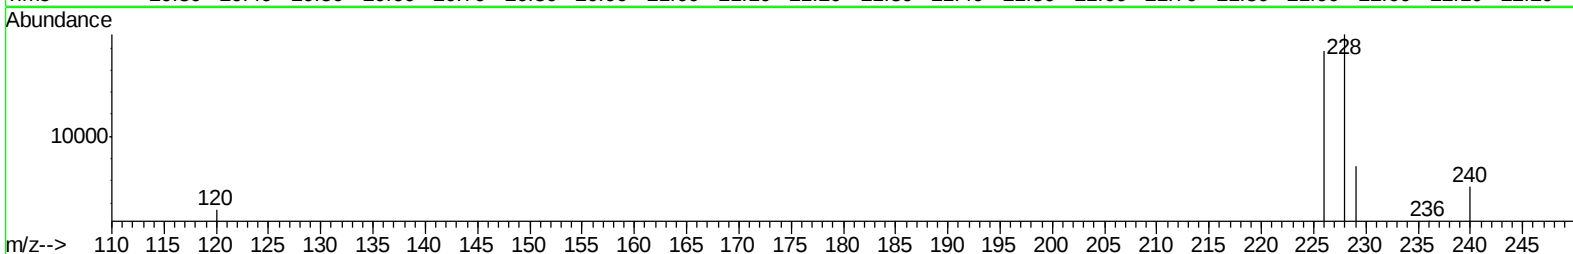


Data File : BM021885.D
Acq On : 07 Aug 2019 08:03
Operator : HP/JU
Sample : K3893-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Aug 07 08:55:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

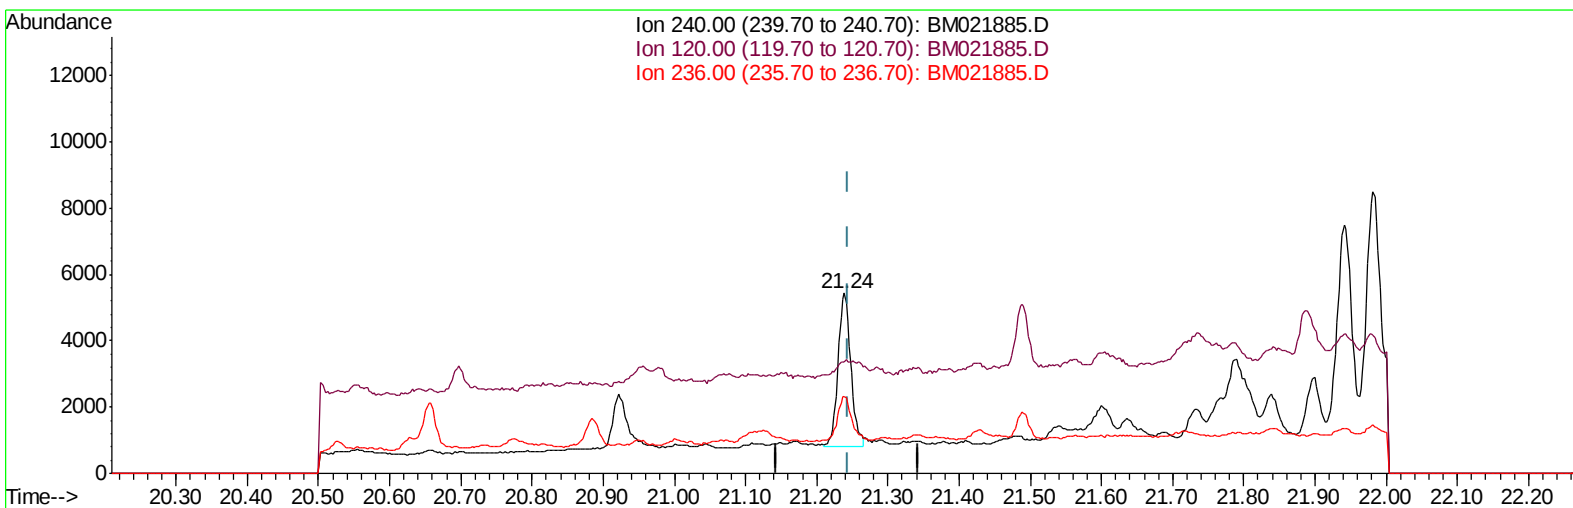

TIC: BM021885.D

(16) Chrysene-d12 (I)

21.239min (-0.005) 0.40ng/ul m

response 5821

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	61.59#
236.00	32.30	42.91#
0.00	0.00	0.00