
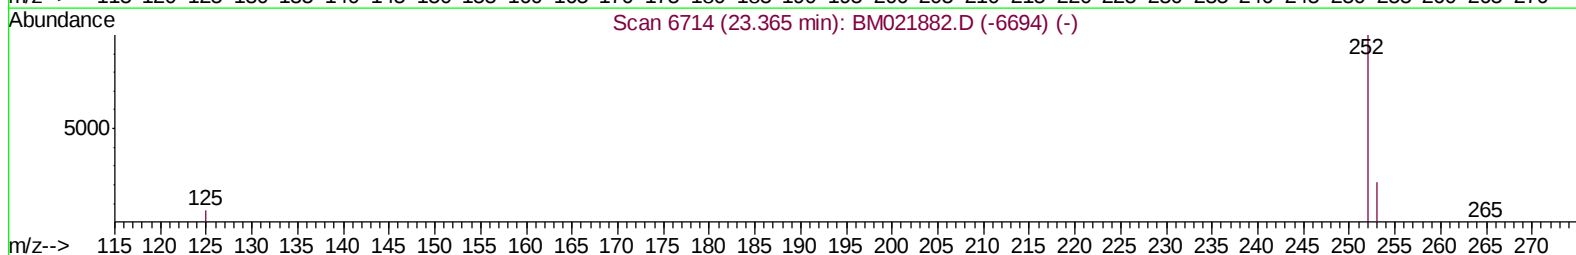
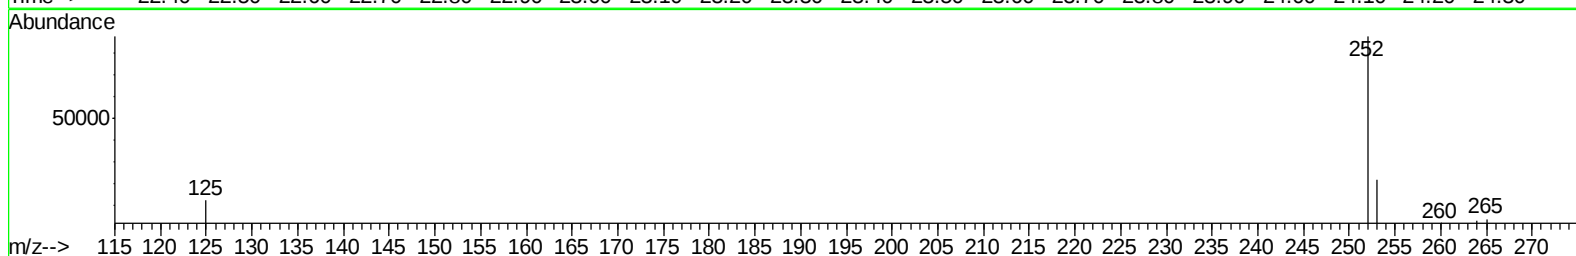


Data File : BM021885.D
Acq On : 07 Aug 2019 08:03
Operator : HP/JU
Sample : K3893-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Aug 07 08:57:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

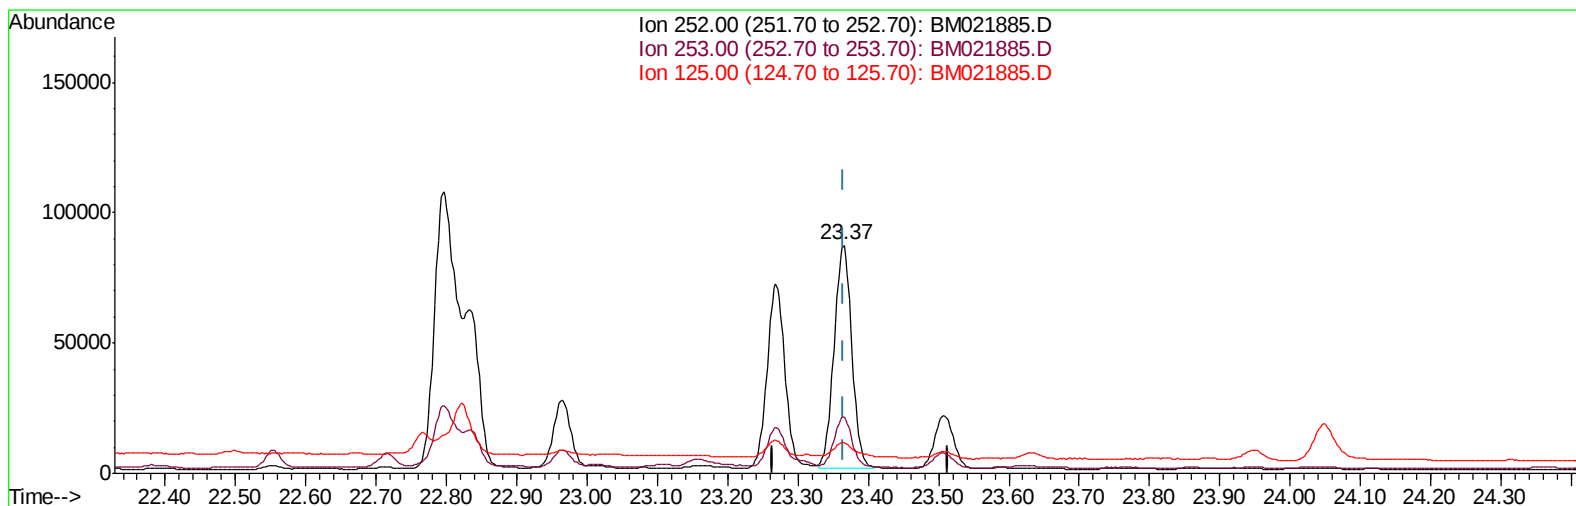

TIC: BM021885.D

(23) Benzo(a)pyrene (C)

23.365min (-0.000) 7.02ng/ul m

response 151705

Ion	Exp%	Act%
252.00	100	100
253.00	39.60	24.71#
125.00	18.20	13.65#
0.00	0.00	0.00