
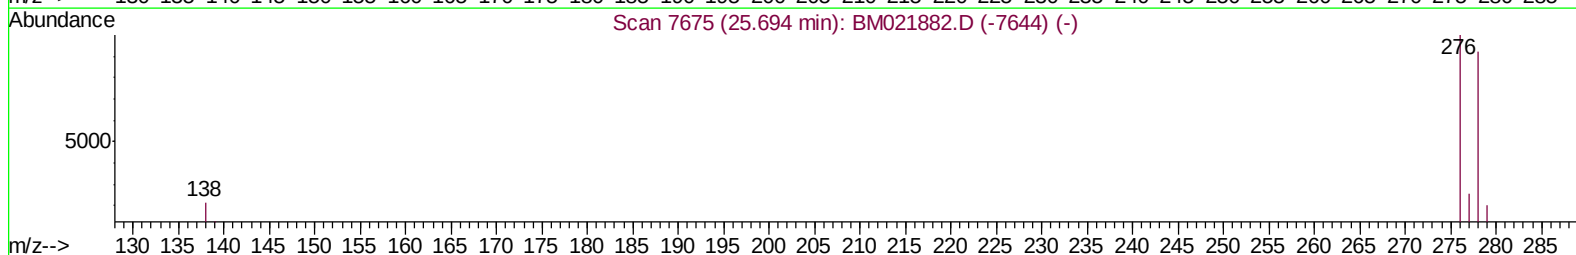
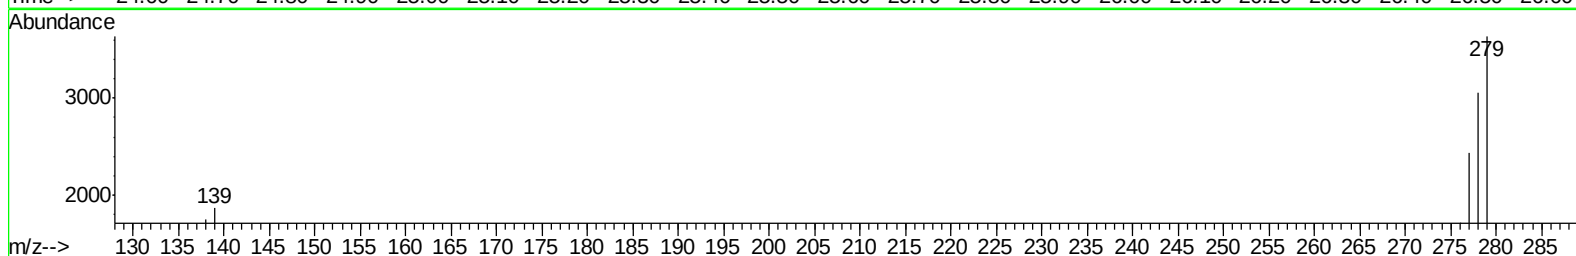


Data File : BM021885.D
Acq On : 07 Aug 2019 08:03
Operator : HP/JU
Sample : K3893-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Aug 07 08:57:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 08:28:11 2019
Response via : Initial Calibration

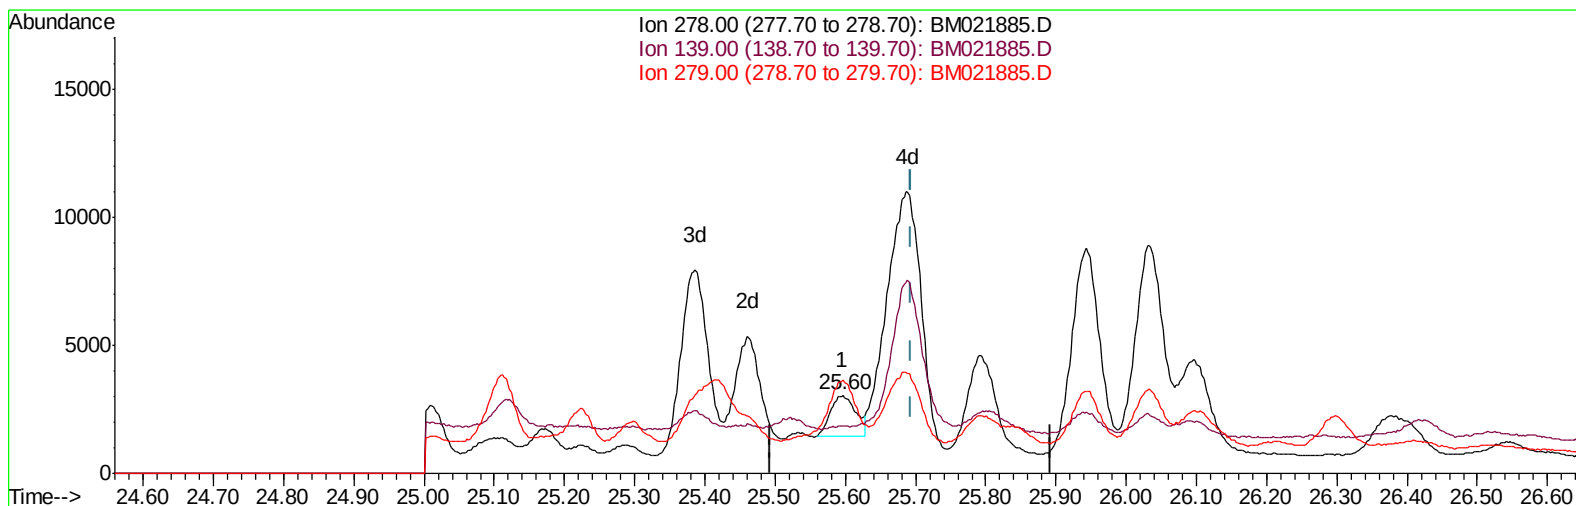

TIC: BM021885.D

(25) Dibenzo(a,h)anthracene

25.597min (-0.097) 0.20ng/ul

response 4139

Ion	Exp%	Act%
278.00	100	100
139.00	17.70	60.81#
279.00	35.40	119.14#
0.00	0.00	0.00