

Data File : BM021881.D
Acq On : 07 Aug 2019 05:01
Operator : HP/JU
Sample : PB121670BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK70

Quant Time: Aug 07 06:00:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1271	0.40	ng/ul	0.00
2) Naphthalene-d8	10.40	136	5407	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	2977	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	552795	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.31	264	691544	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	2703	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.28	166	980	0.078	ng/ul#	Qvalue 17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021881.D
Acq On : 07 Aug 2019 05:01
Operator : HP/JU
Sample : PB121670BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK70

Quant Time: Aug 07 06:00:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration

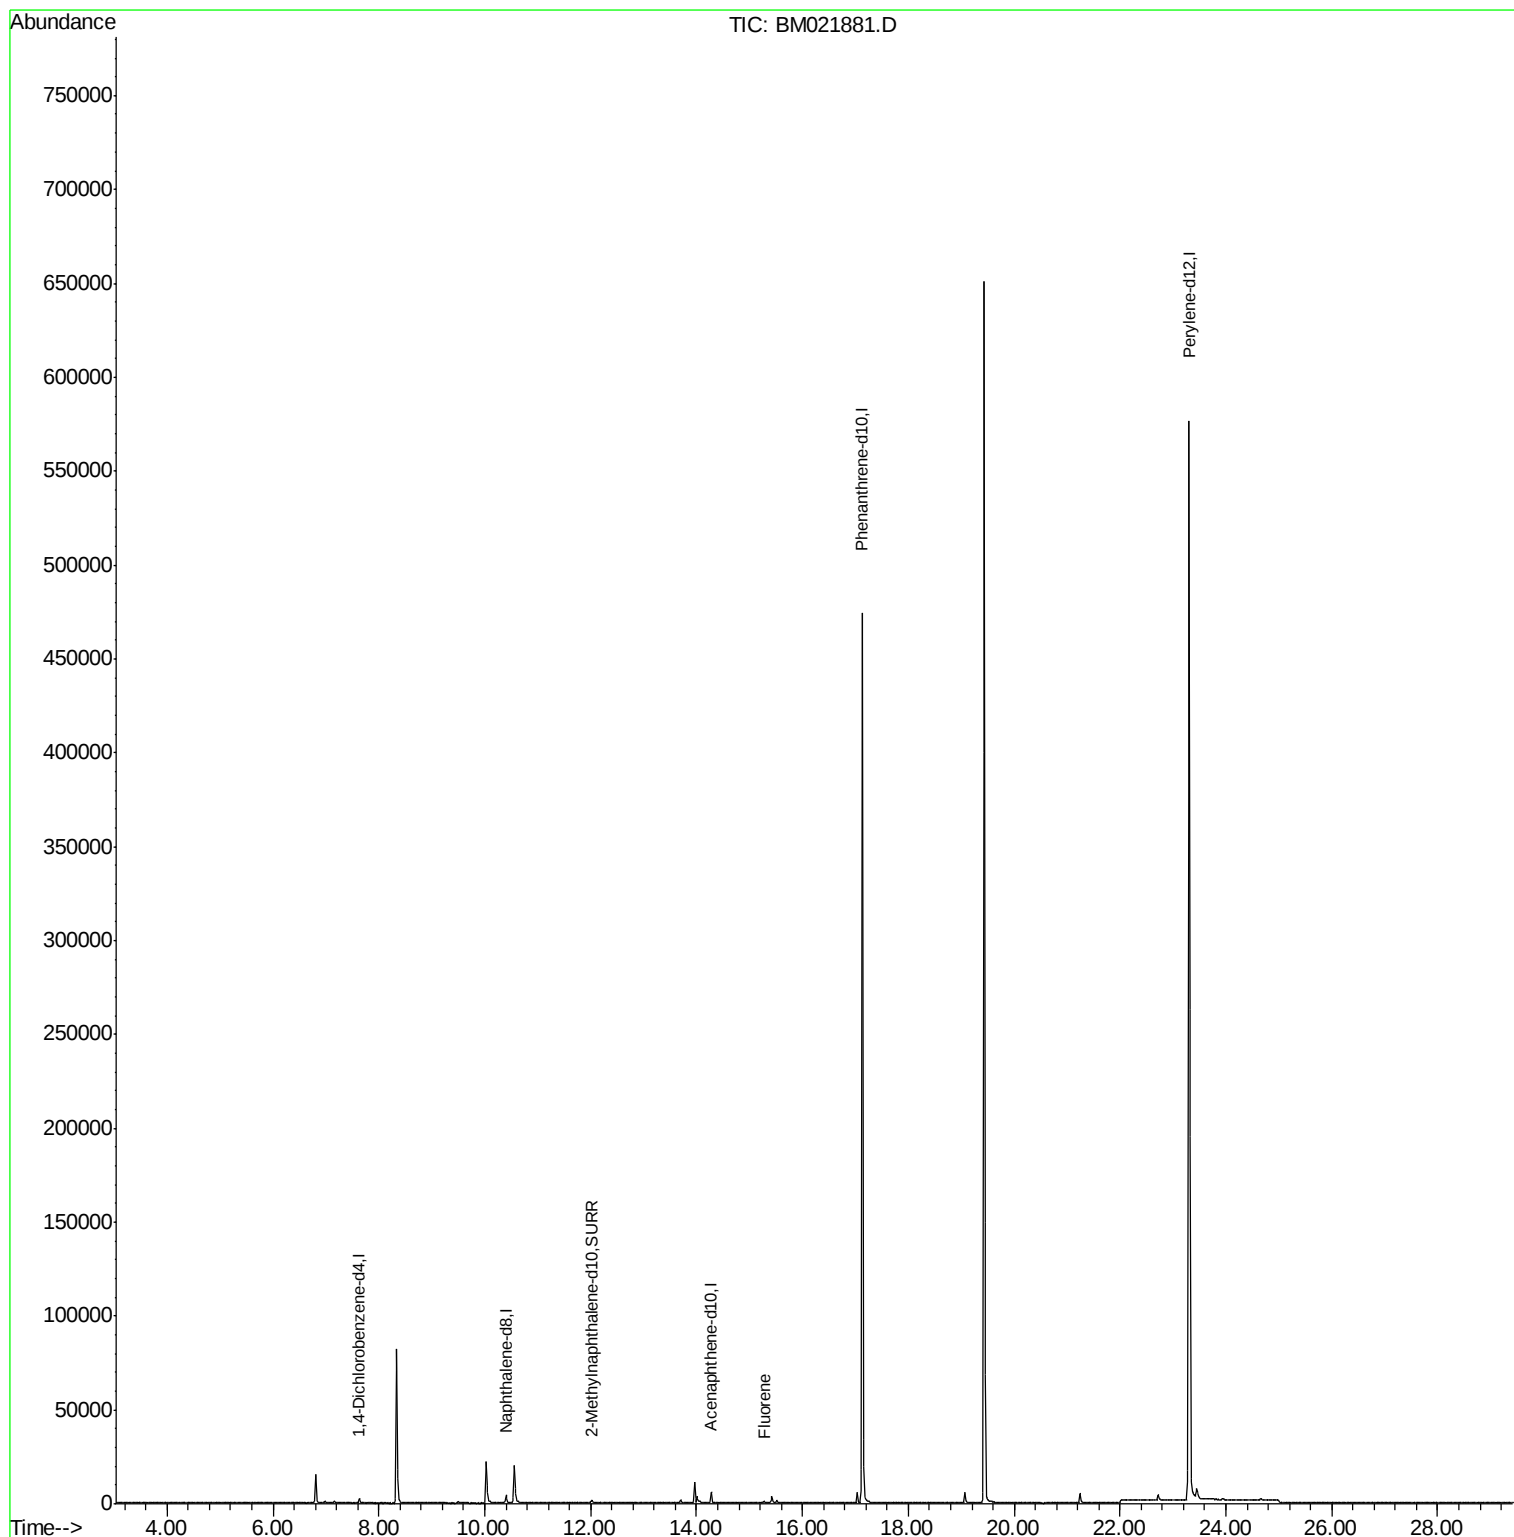

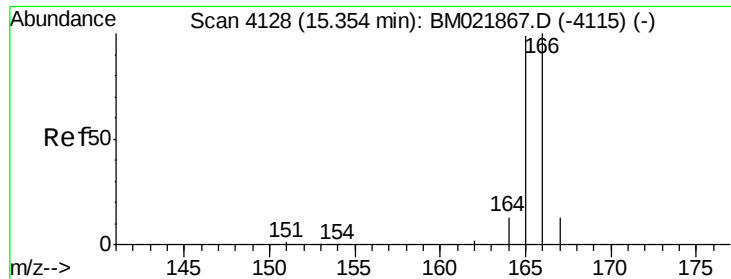

#9

Fluorene

Concen: 0.078 ng/ul

RT: 15.28 min Scan# 4108

Delta R.T. -0.08 min

Lab File: BM021881.D


Acq: 07 Aug 2019 05:01

Instrument :

BNA_M

ClientSampleId :

SBLK70

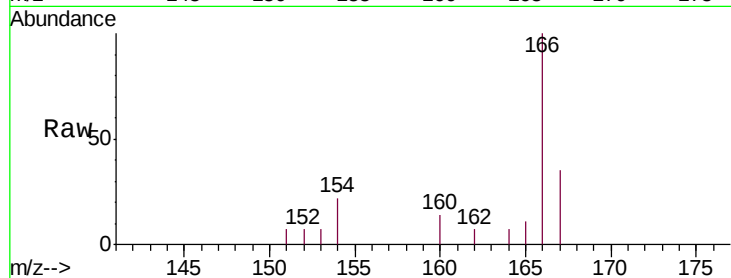


Tgt Ion:166 Resp: 980

Ion Ratio Lower Upper

166 100

165 10.7 81.4 122.0#

167 34.9 13.7 20.5#

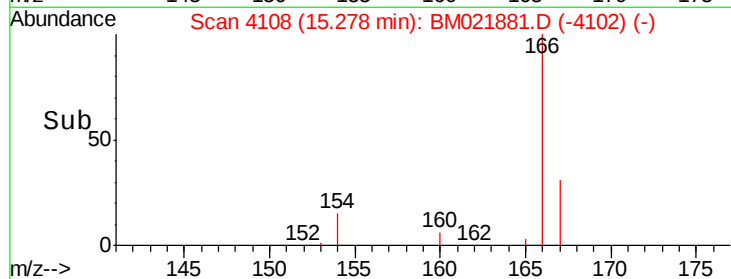

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

