

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080619\
Quantitation Report (QT Reviewed)


Data File : BM021870.D
Acq On : 06 Aug 2019 22:20
Operator : HP/JU
Sample : K3922-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F0MSD

Manual Integrations
APPROVED

mohammad
8/7/2019 12:12:17 PM

Quant Time: Aug 07 04:21:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration

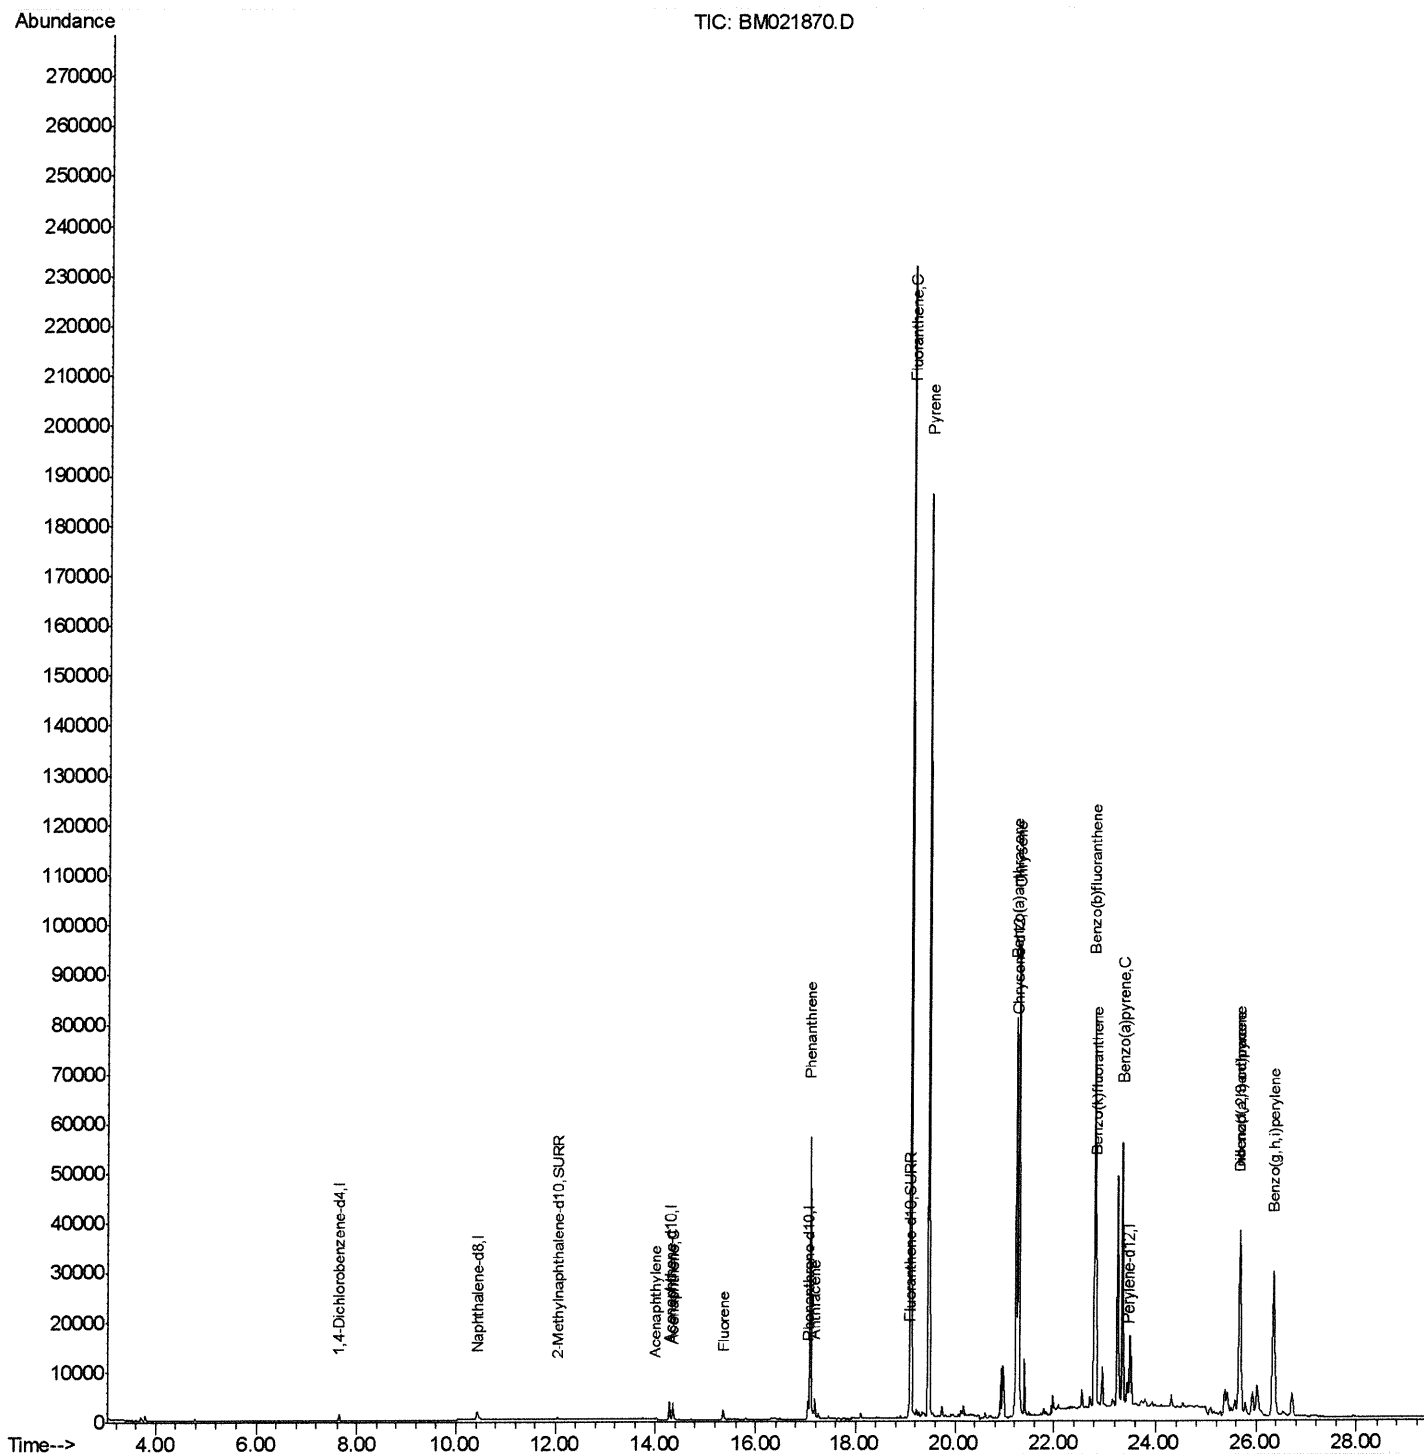

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080619\
Quantitation Report (Qedit)




Data File : BM021870.D
Acq On : 06 Aug 2019 22:20
Operator : HP/JU
Sample : K3922-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F0MSD

Manual Integrations
APPROVED

mohammad
8/7/2019 12:12:17 PM

Quant Time: Aug 07 04:05:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration

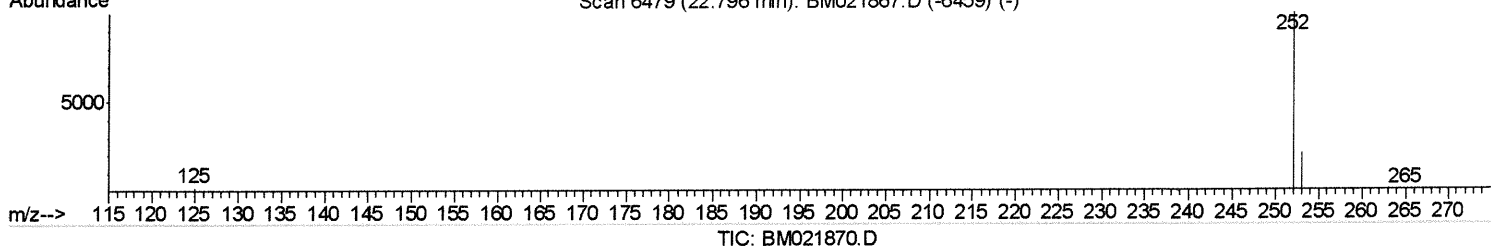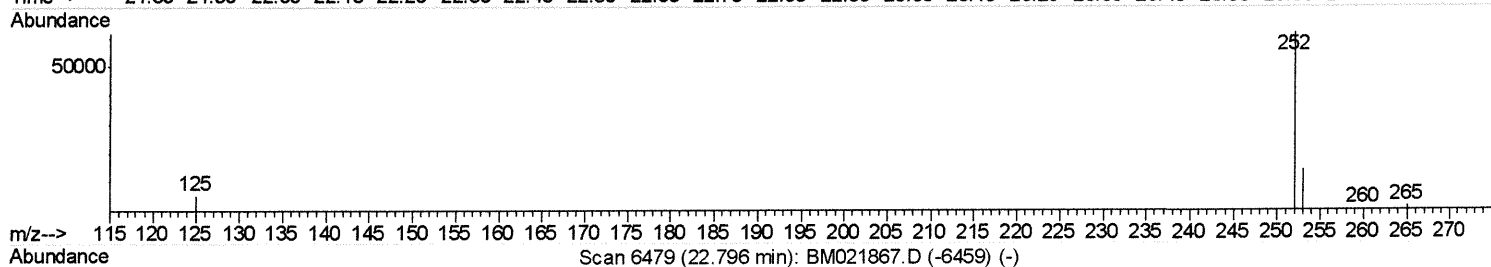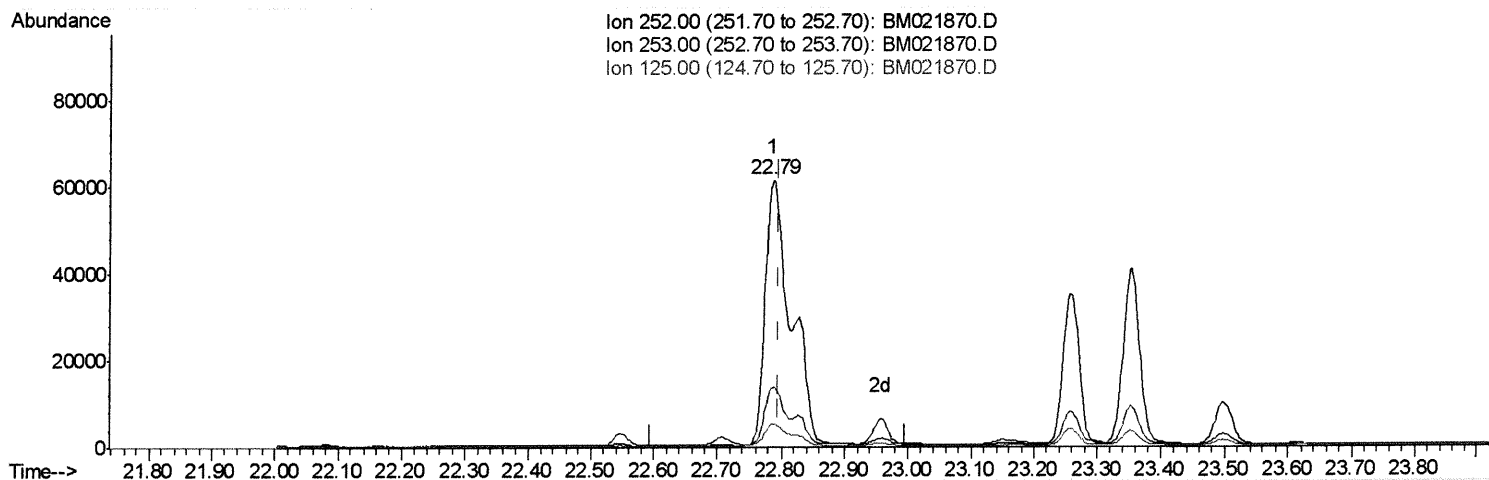

(21) Benzo(b)fluoranthene
22.786min (-0.009) 7.85ng/ul
response 172779

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	22.71
125.00	15.50	8.58
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080619\
Quantitation Report (Qedit)



Data File : BM021870.D
Acq On : 06 Aug 2019 22:20
Operator : HP/JU
Sample : K3922-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F0MSD

Manual Integrations
APPROVED

mohammad
8/7/2019 12:12:17 PM

Quant Time: Aug 07 04:05:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration

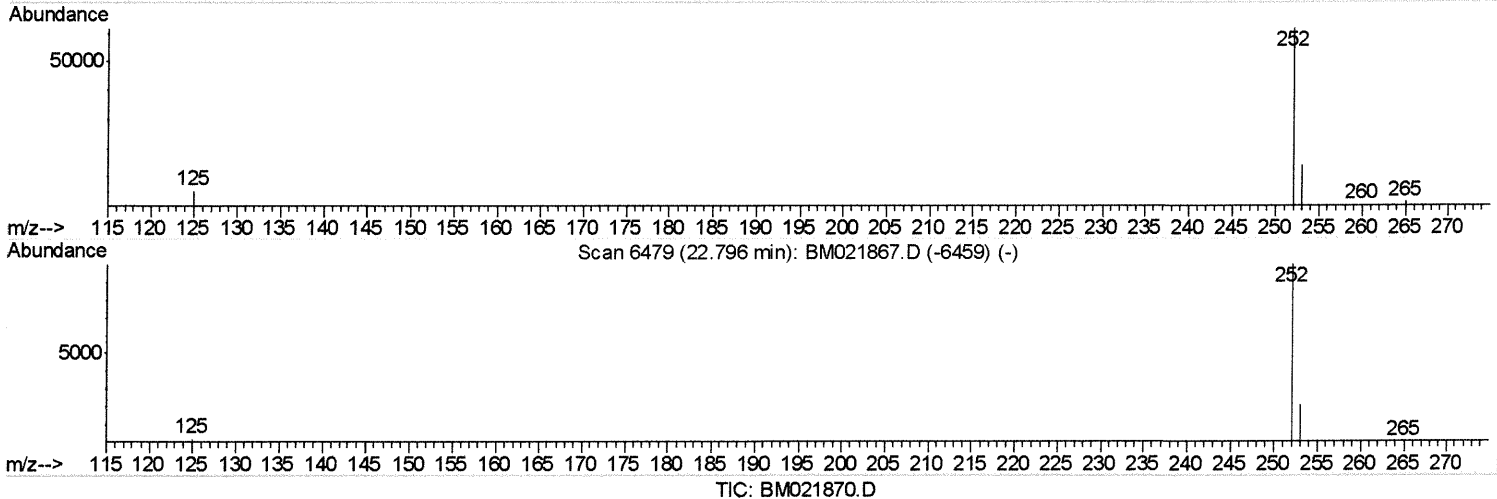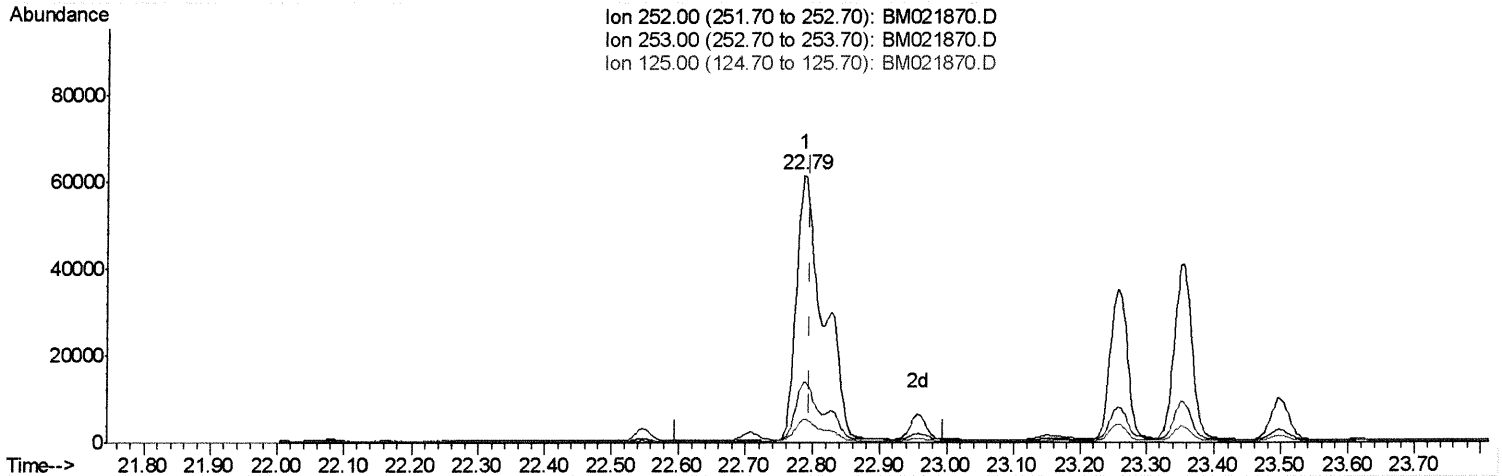

(21) Benzo(b)fluoranthene

22.786min (-0.009) 5.63ng/ul m

response 123933

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	22.71
125.00	15.50	8.58
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080619\
Quantitation Report (Qedit)



Data File : BM021870.D
Acq On : 06 Aug 2019 22:20
Operator : HP/JU
Sample : K3922-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F0MSD

Manual Integrations
APPROVED

mohammad
8/7/2019 12:12:17 PM

Quant Time: Aug 07 04:05:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration

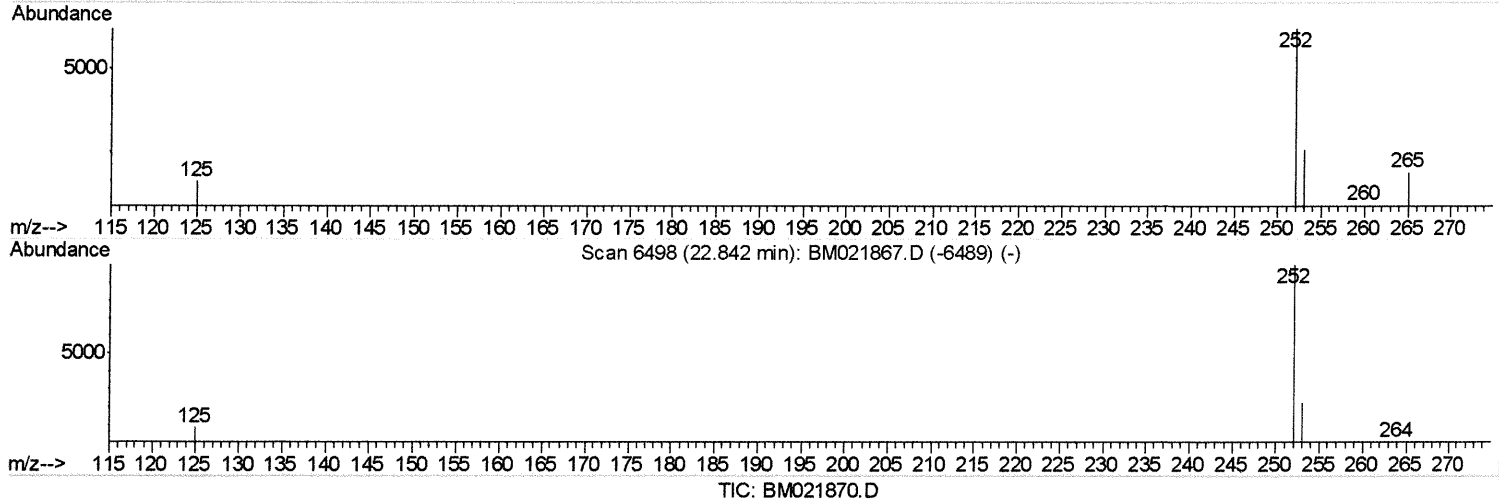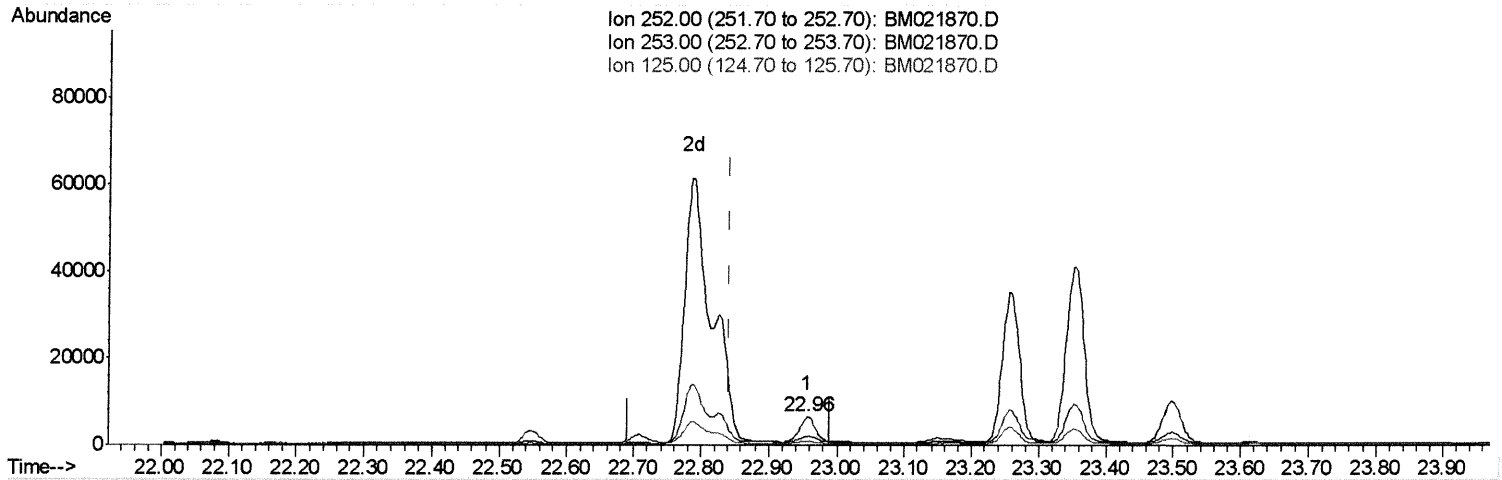

(22) Benzo(k)fluoranthene
22.956min (+0.114) 0.34ng/ul
response 8512

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	32.72
125.00	15.20	14.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080619\
Quantitation Report (Qedit)




Data File : BM021870.D
Acq On : 06 Aug 2019 22:20
Operator : HP/JU
Sample : K3922-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F0MSD

Manual Integrations
APPROVED

mohammad
8/7/2019 12:12:17 PM

Quant Time: Aug 07 04:05:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 07 04:02:33 2019
Response via : Initial Calibration

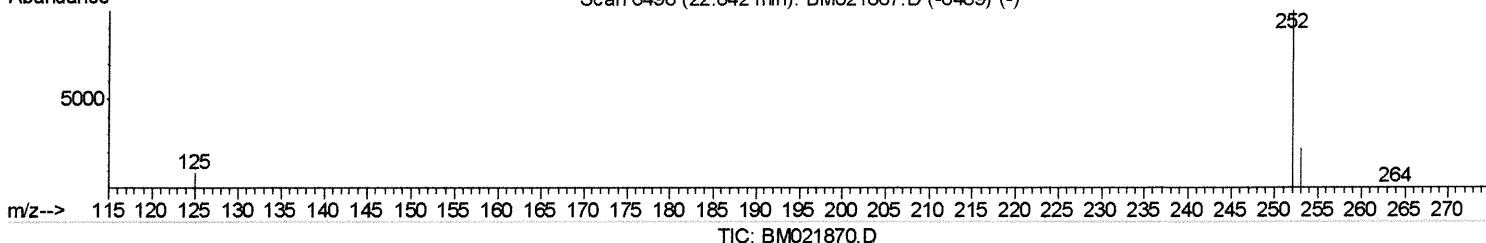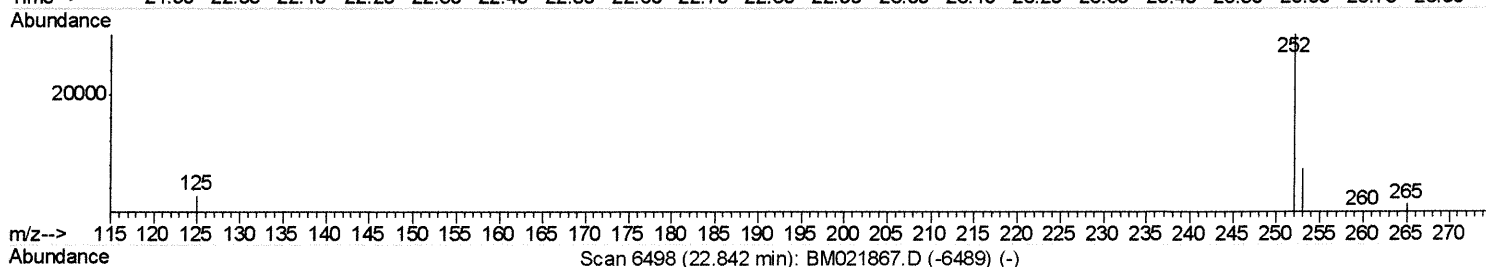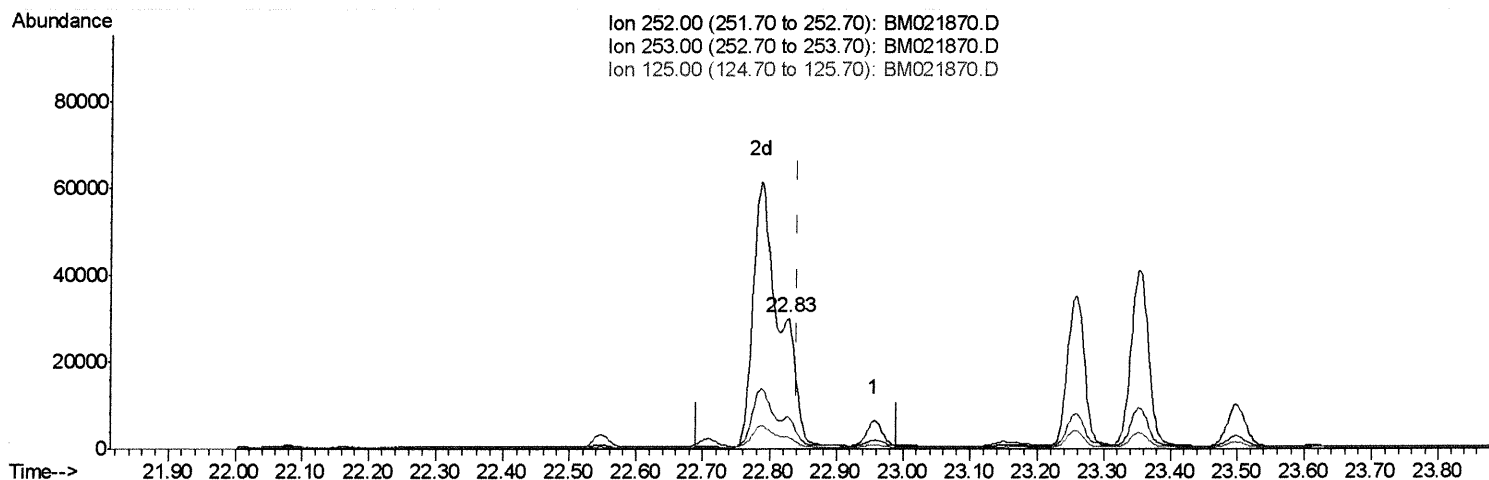

(22) Benzo(k)fluoranthene

22.827min (-0.014) 1.91ng/ul m

JU
08/07/19

response 47677

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.94#
125.00	15.20	9.36#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080619\
 Quantitation Report (QT Reviewed)
 Data File : BM021870.D
 Acq On : 06 Aug 2019 22:20
 Operator : HP/JU
 Sample : K3922-03MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F0MSD

Manual Integrations
 APPROVED

mohammad
 8/7/2019 12:12:17 PM

Quant Time: Aug 07 04:21:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 07 04:02:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	843	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	3651	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	2121	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	4902	0.40	ng/ul	-0.01
16) Chrysene-d12	21.23	240	5068	0.40	ng/ul	-0.01
20) Perylene-d12	23.45	264	6524	0.40	ng/ul	-0.01

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	896	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	2602	0.16	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.01	152	728	0.074	ng/ul#	81
8) Acenaphthene	14.35	153	2110	0.261	ng/ul	97
9) Fluorene	15.35	166	1347	0.150	ng/ul	97
12) Phenanthrene	17.08	178	62902	4.410	ng/ul	96
13) Anthracene	17.18	178	4522	0.372	ng/ul	100
15) Fluoranthene	19.10	202	197513	10.338	ng/ul	97
17) Pyrene	19.47	202	160856	7.724	ng/ul	100
18) Benzo(a)anthracene	21.22	228	66148	3.649	ng/ul	99
19) Chrysene	21.27	228	94312	4.045	ng/ul	100
21) Benzo(b)fluoranthene	22.79	252	123933m →	5.633	ng/ul	3 Ju 08/07/19
22) Benzo(k)fluoranthene	22.83	252	47677m →	1.915	ng/ul	
23) Benzo(a)pyrene	23.35	252	75153	3.359	ng/ul#	75
24) Indeno(1,2,3-cd)pyrene	25.66	276	63897	2.392	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.67	278	13702	0.635	ng/ul	92
26) Benzo(g,h,i)perylene	26.34	276	61333	2.550	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed