

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080619\
 Data File : BM021860.D
 Acq On : 06 Aug 2019 09:49
 Operator : HP/JU
 Sample : K3890-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52Q6

Manual Integrations
 APPROVED

mohammad
 8/6/2019 10:22:05 PM

Quant Time: Aug 06 11:21:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 06 01:29:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	809	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	3358	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.28	164	1903	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	4479m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.25	240	4047m	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	3696m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	1507	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	4557m	0.30	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.46	128	359	0.038	ng/ul#	Ovalue 62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080619\
Data File : BM021860.D
Acq On : 06 Aug 2019 09:49
Operator : HP/JU
Sample : K3890-10
Misc :
ALS Vial : 4 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A52Q6

Manual Integrations
APPROVED

mohammad
8/6/2019 10:22:05 PM

Quant Time: Aug 06 11:21:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

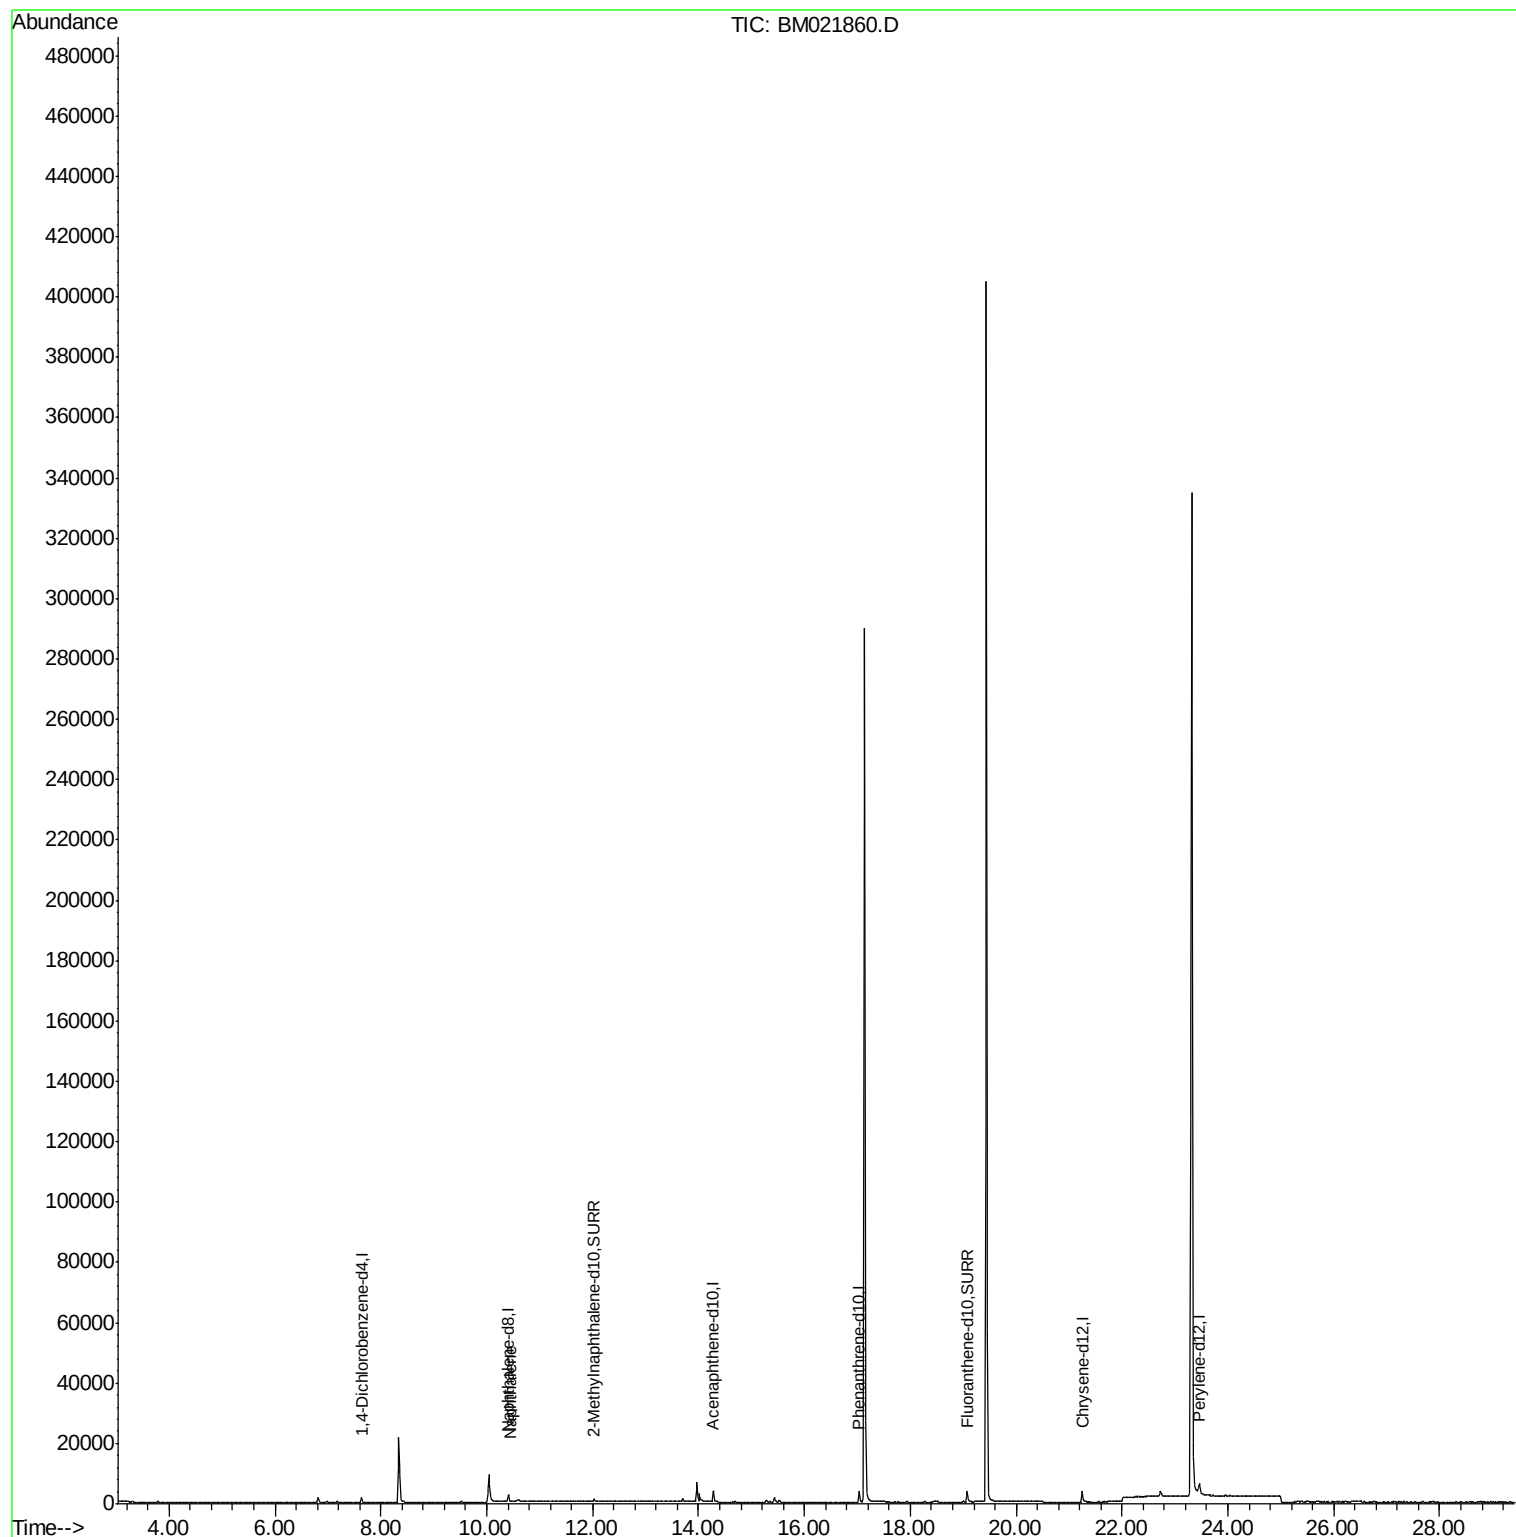

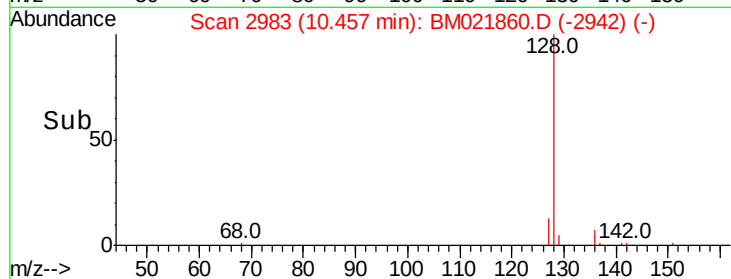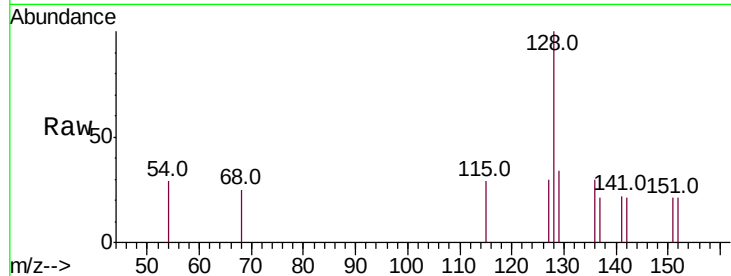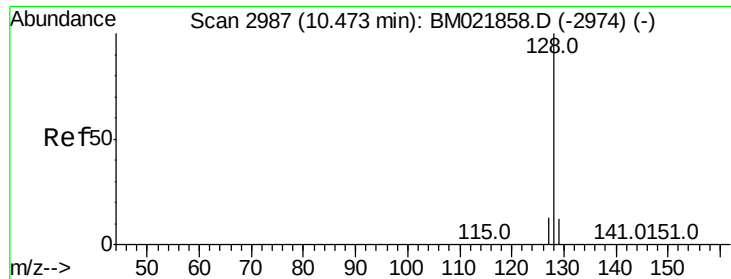

#3

Naphthalene

Concen: 0.038 ng/ul

RT: 10.46 min Scan# 2983

Delta R.T. -0.01 min

Lab File: BM021860.D

Acq: 06 Aug 2019 09:49

Instrument :

BNA_M

ClientSampleId :

A52Q6

Tot Ion:	128	Resp:	359
Ion Ratio	Lower	Upper	
128	100		
129	33.6	12.3	18.5#
127	30.5	13.0	19.6#

Manual Integrations
APPROVED

mohammad
8/6/2019 10:22:05 PM

