
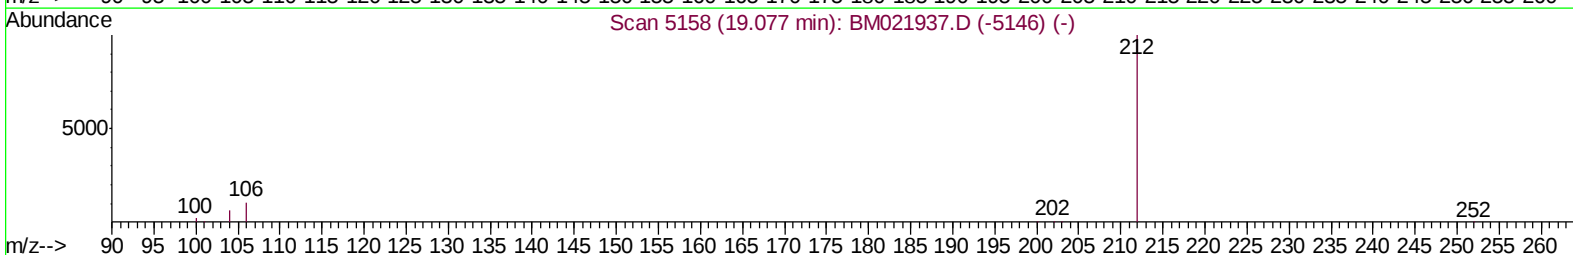
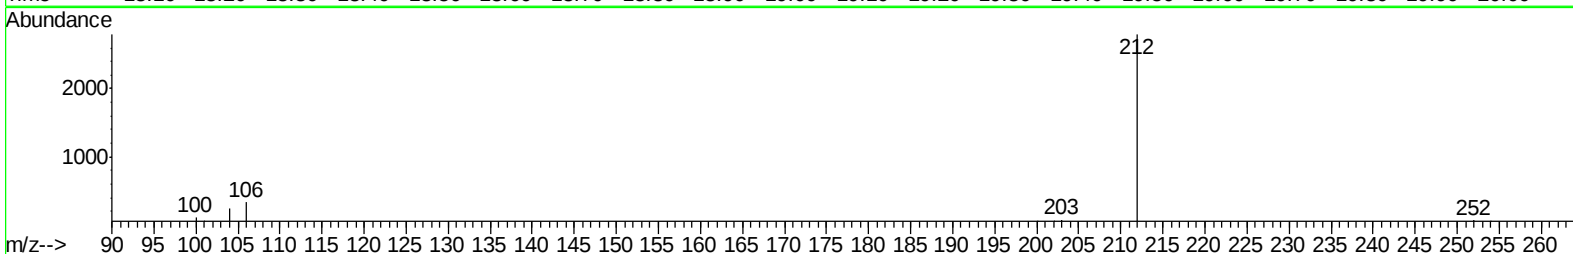


Data File : BM021938.D
Acq On : 08 Aug 2019 18:06
Operator : HP/JU
Sample : PB121849BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Quant Time: Aug 09 01:35:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

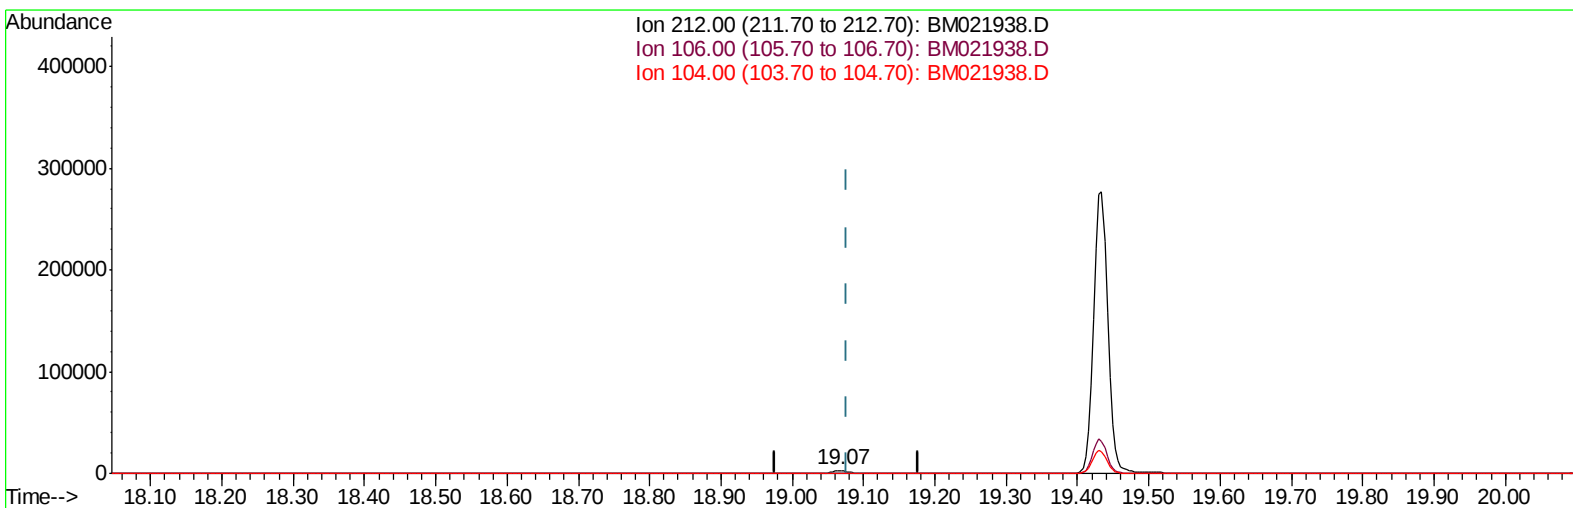

TIC: BM021938.D

(14) Fluoranthene-d10 (SURR)

19.068min (-0.009) 0.36ng/ul m

response 3877

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00