
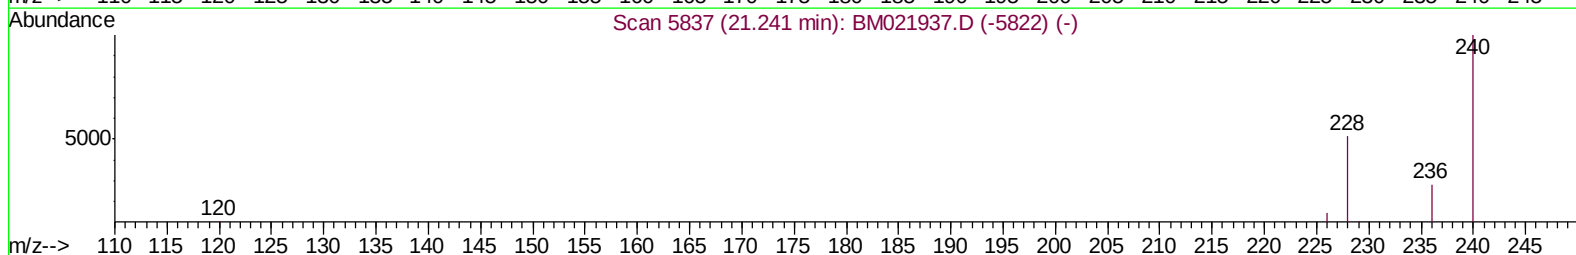
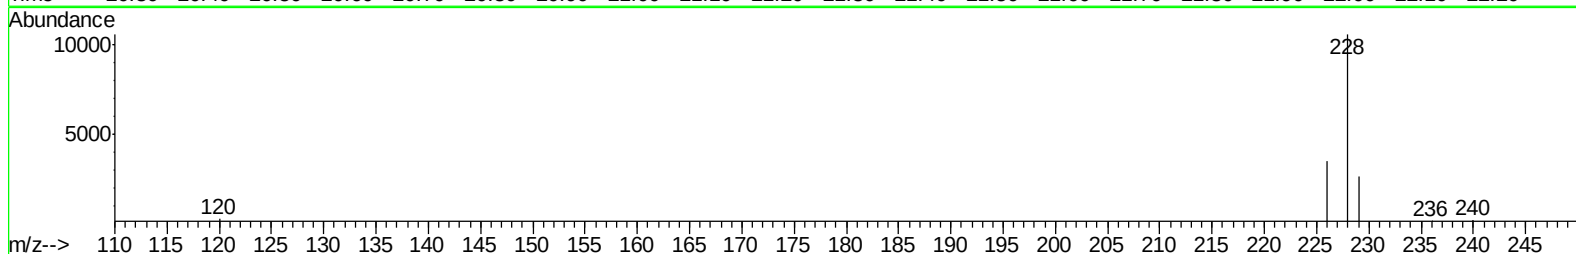


Data File : BM021939.D
Acq On : 08 Aug 2019 18:43
Operator : HP/JU
Sample : K4029-18
Misc :
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Aug 09 01:41:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

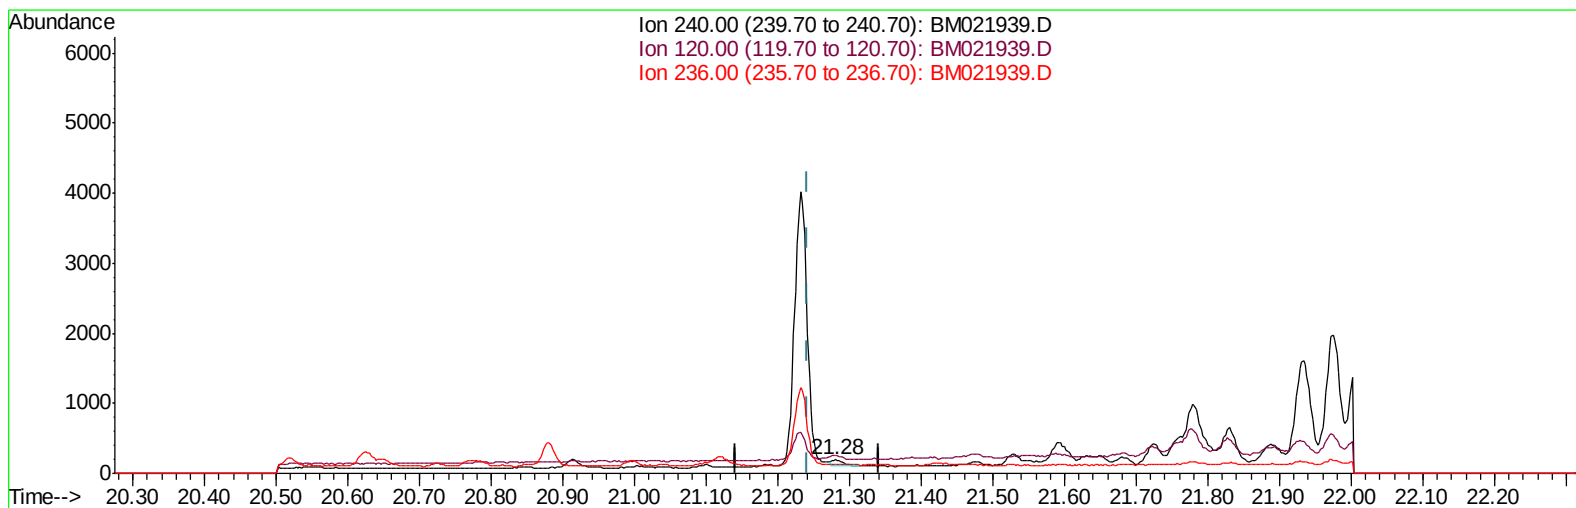

TIC: BM021939.D

(16) Chrysene-d12 (I)

21.280min (+0.039) 0.40ng/ul

response 92

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	126.90#
236.00	32.30	64.97#
0.00	0.00	0.00