
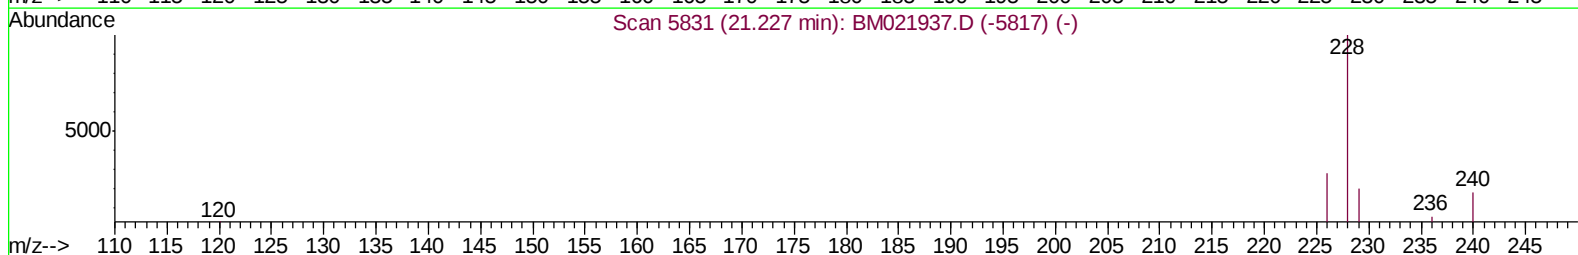
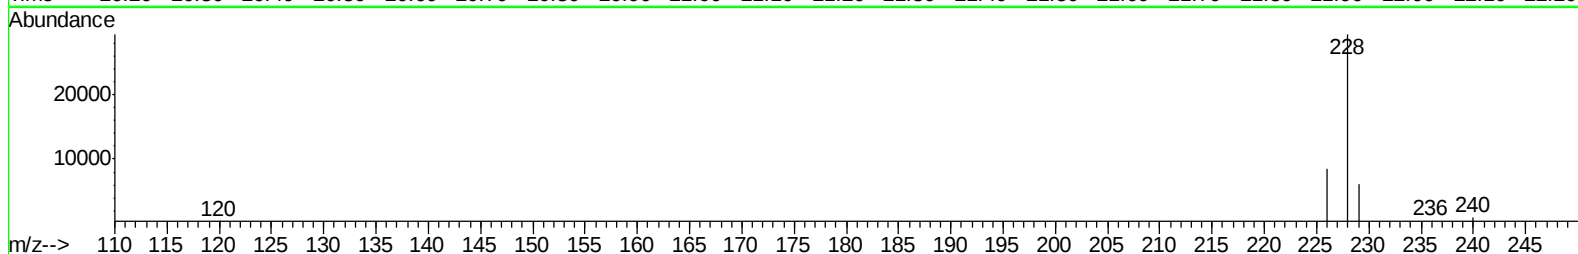


Data File : BM021939.D
Acq On : 08 Aug 2019 18:43
Operator : HP/JU
Sample : K4029-18
Misc :
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Aug 09 01:42:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

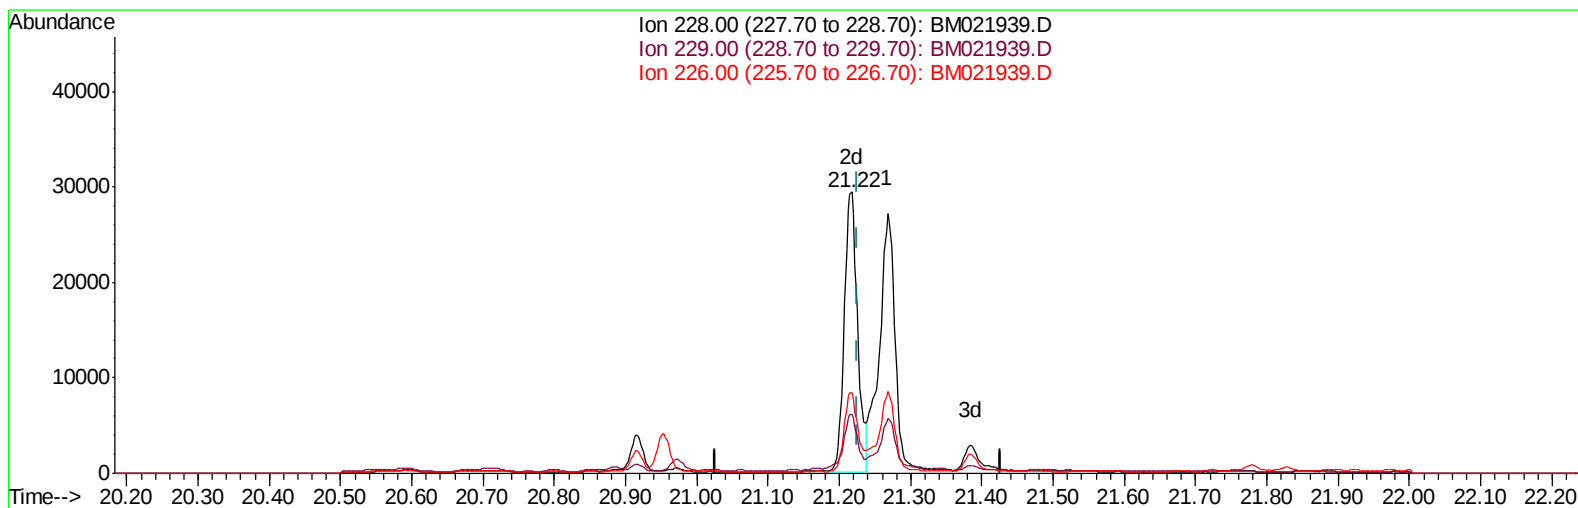

TIC: BM021939.D

(18) Benzo(a)anthracene
21.217min (-0.009) 2.21ng/ul m
response 38153

Ion	Exp%	Act%
228.00	100	100
229.00	21.50	21.03
226.00	28.30	28.84
0.00	0.00	0.00