
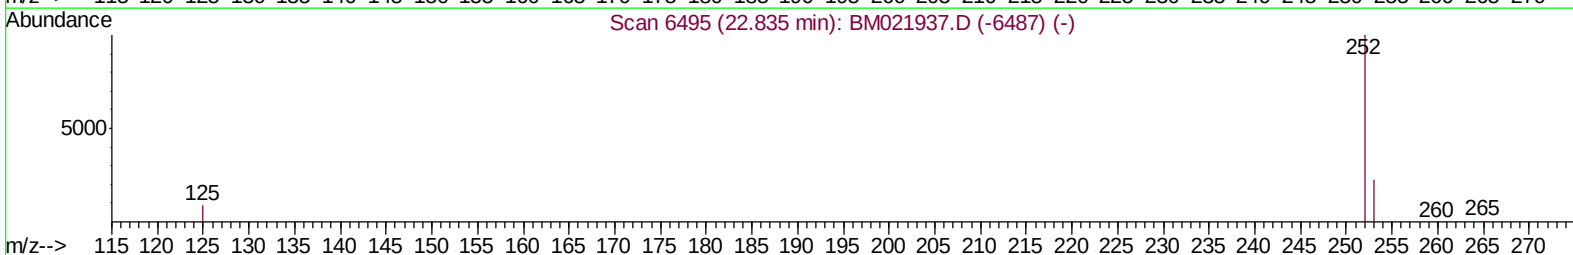
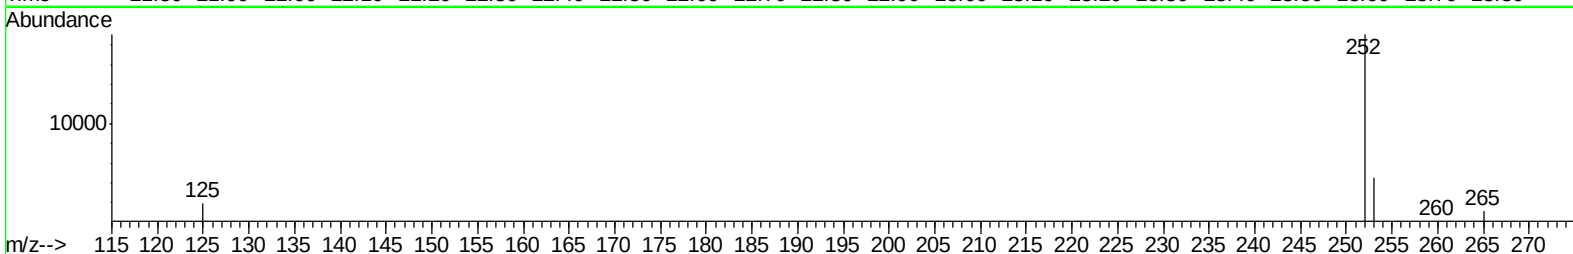


Data File : BM021939.D
Acq On : 08 Aug 2019 18:43
Operator : HP/JU
Sample : K4029-18
Misc :
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Aug 09 01:43:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

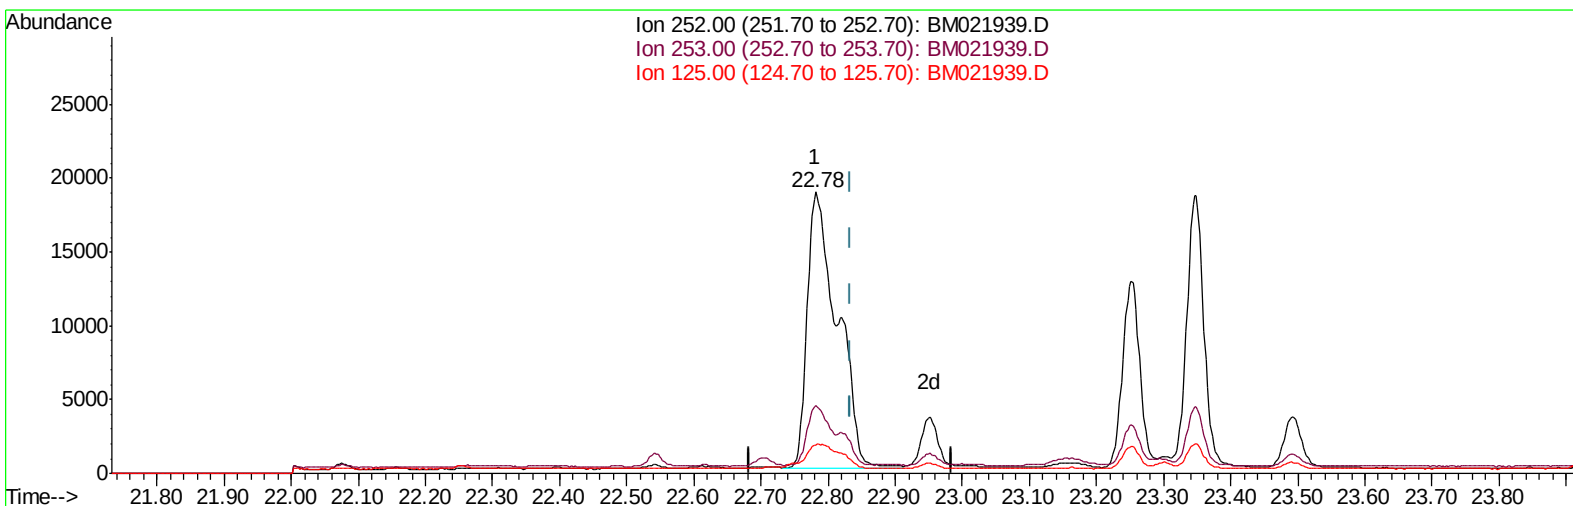

TIC: BM021939.D

(22) Benzo(k)fluoranthene
22.781min (-0.053) 3.13ng/ul
response 57770

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.01#
125.00	15.20	10.10#
0.00	0.00	0.00