
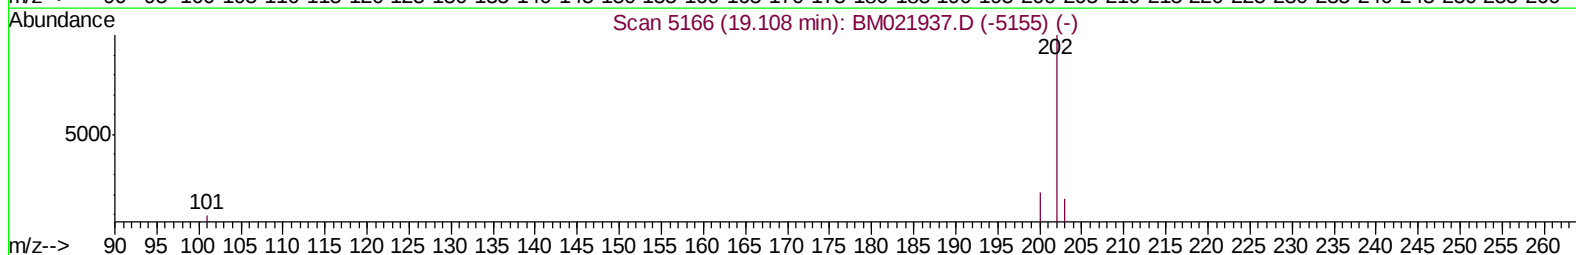
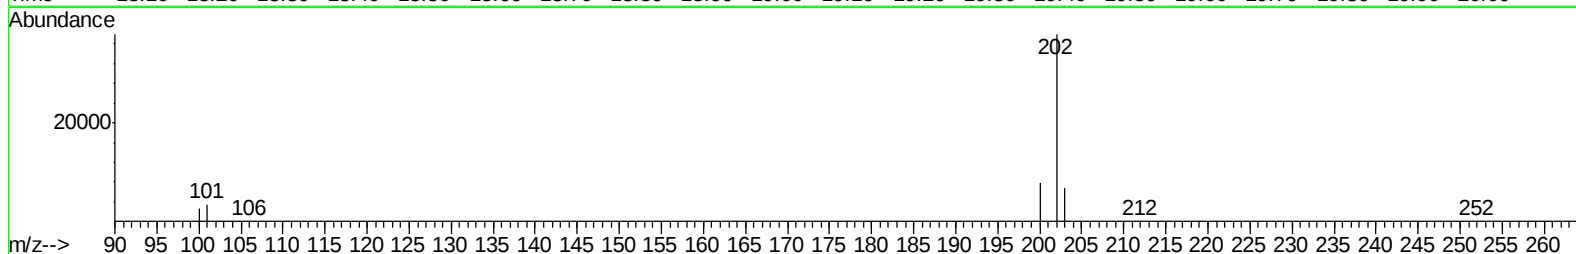


Data File : BM021940.D
Acq On : 08 Aug 2019 19:20
Operator : HP/JU
Sample : K4029-19
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 09 01:46:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

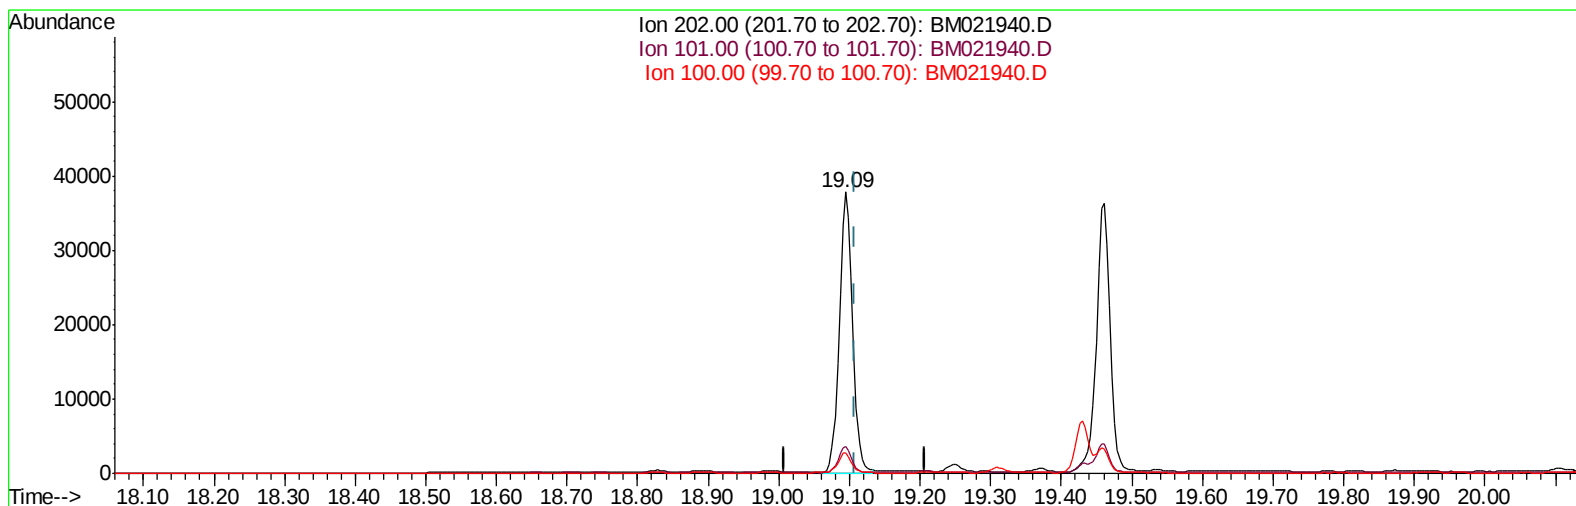

TIC: BM021940.D

(15) Fluoranthene (C)

19.095min (-0.013) 2.49ng/ul m

response 49688

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	9.34
100.00	8.10	7.17
0.00	0.00	0.00