
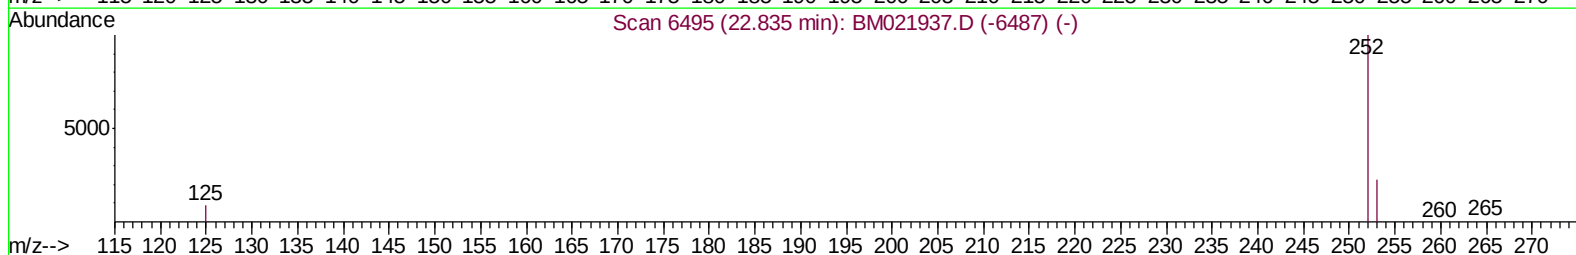
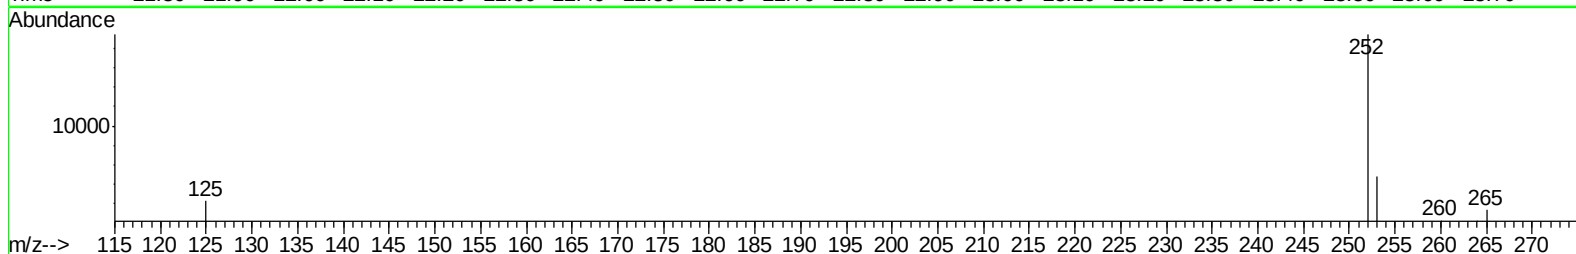


Data File : BM021940.D
Acq On : 08 Aug 2019 19:20
Operator : HP/JU
Sample : K4029-19
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 09 01:48:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

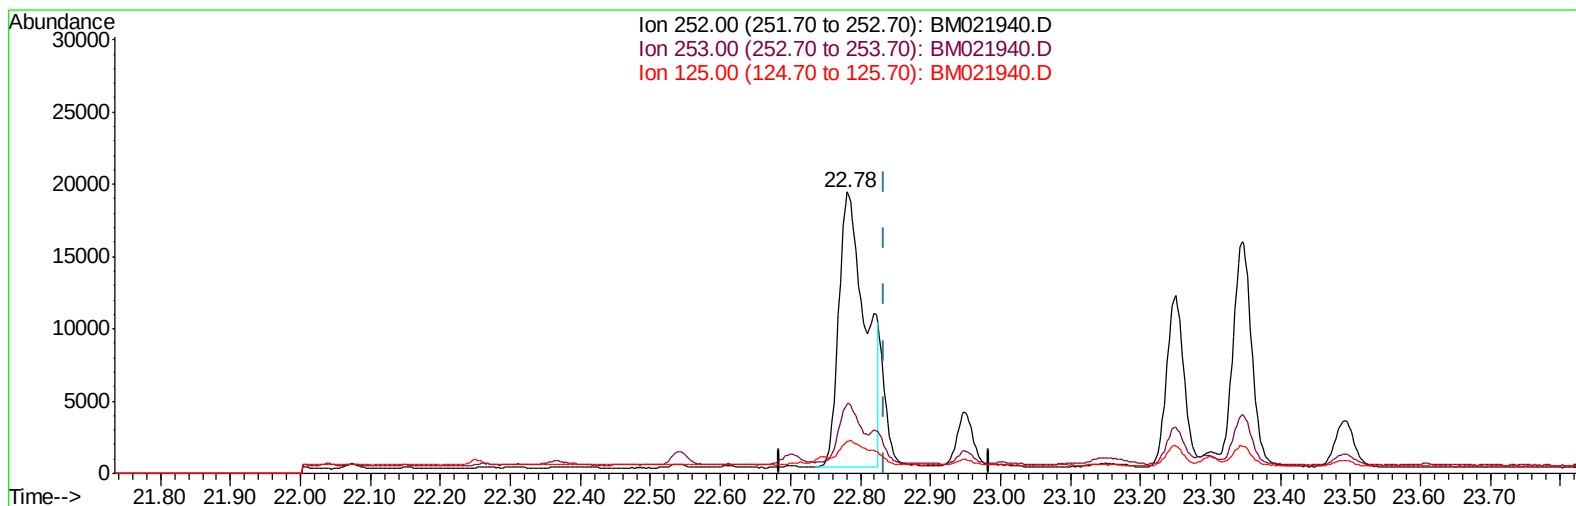

TIC: BM021940.D

(22) Benzo(k)fluoranthene
22.781min (-0.054) 2.47ng/ul
response 49836

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.56#
125.00	15.20	11.32#
0.00	0.00	0.00