
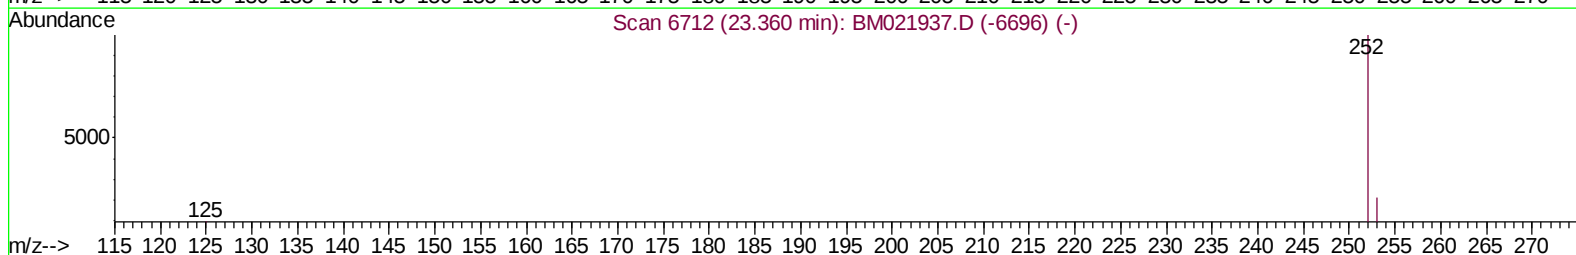
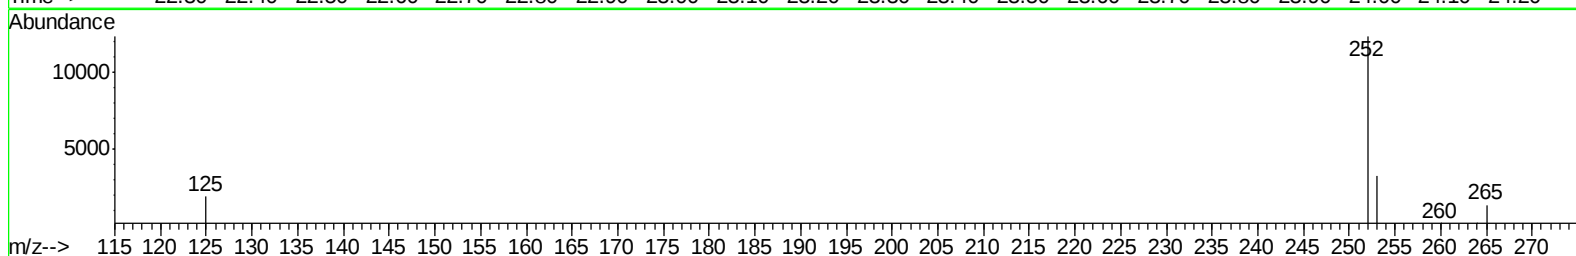


Data File : BM021940.D  
Acq On : 08 Aug 2019 19:20  
Operator : HP/JU  
Sample : K4029-19  
Misc :  
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 09 01:48:35 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 09 01:29:50 2019  
Response via : Initial Calibration

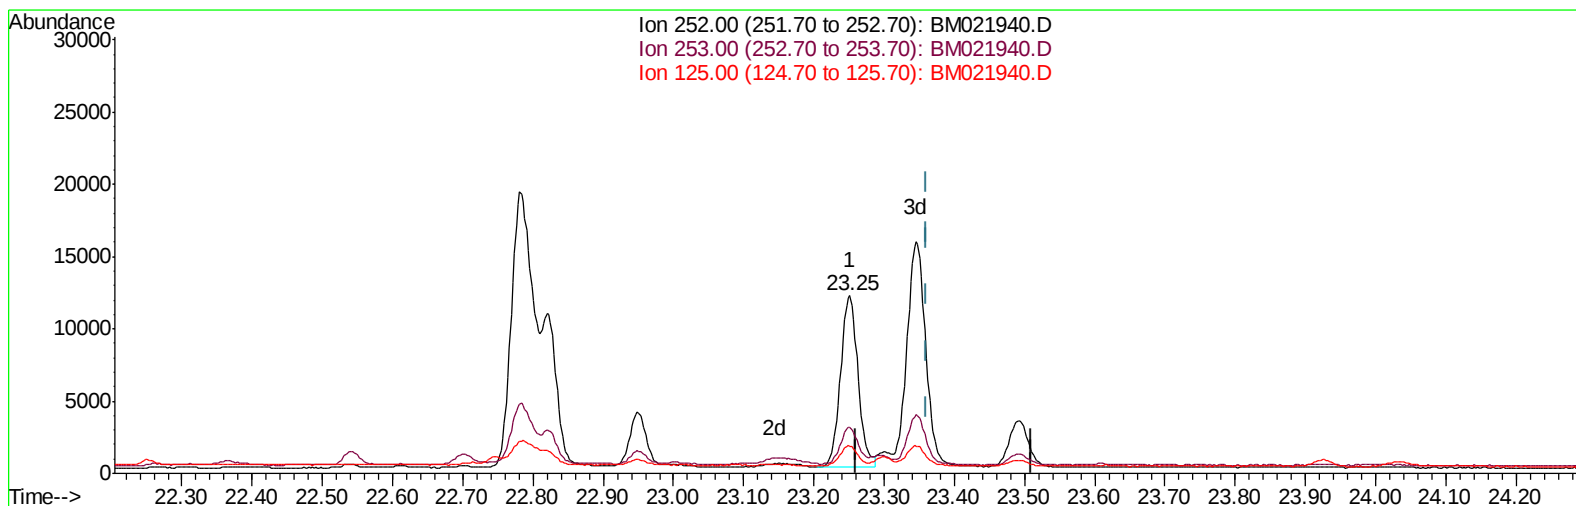

TIC: BM021940.D

(23) Benzo(a)pyrene (C)  
23.251min (-0.109) 1.14ng/ul  
response 20667

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 39.60 | 25.93# |
| 125.00 | 18.20 | 15.35  |
| 0.00   | 0.00  | 0.00   |