
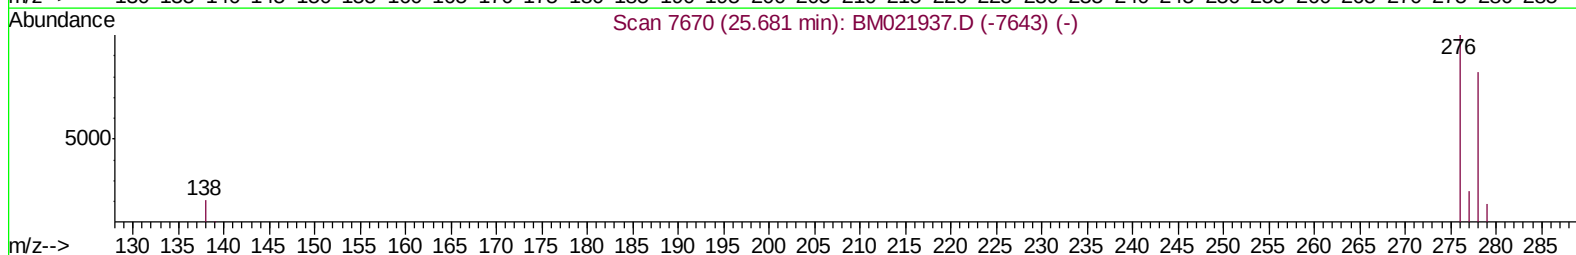
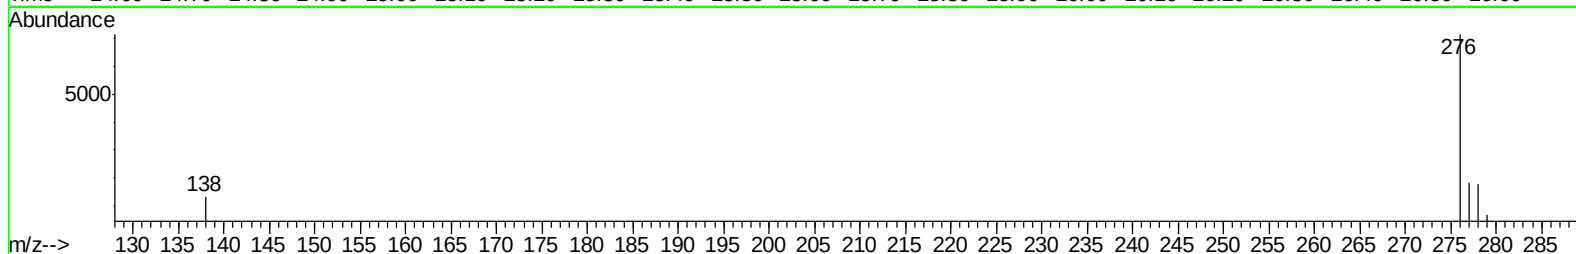


Data File : BM021940.D  
Acq On : 08 Aug 2019 19:20  
Operator : HP/JU  
Sample : K4029-19  
Misc :  
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 09 01:48:35 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 09 01:29:50 2019  
Response via : Initial Calibration

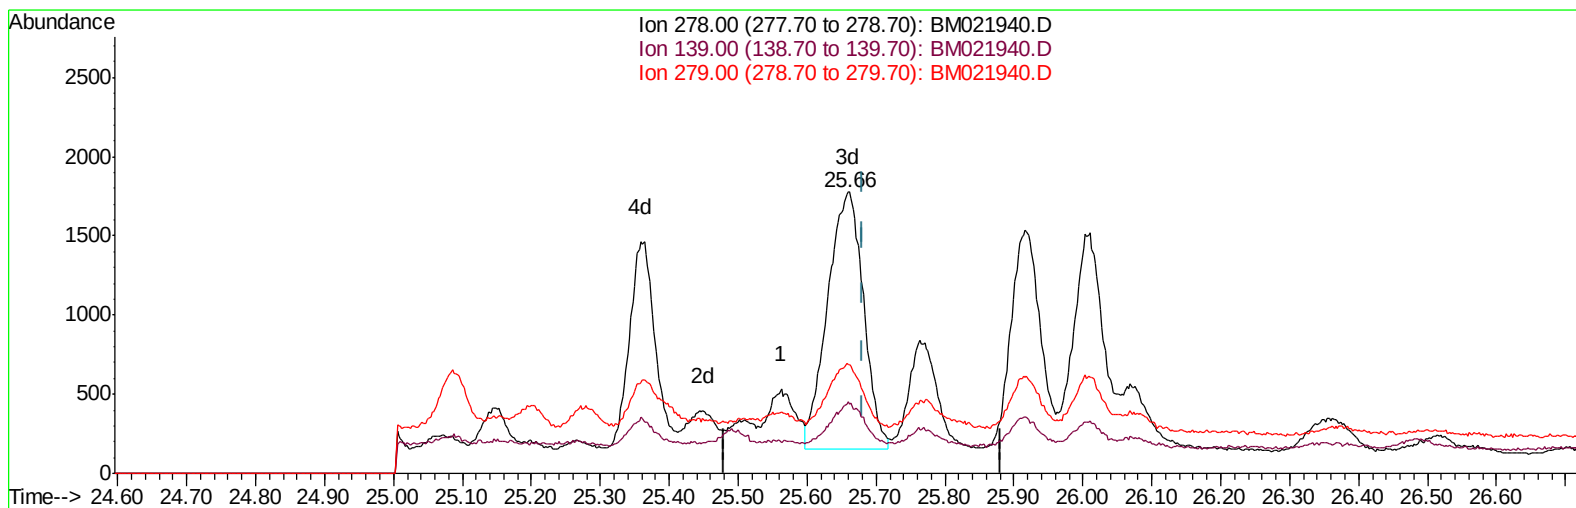

TIC: BM021940.D

(25) Dibenzo(a,h)anthracene

25.659min (-0.022) 0.34ng/ul m

response 5893

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 278.00 | 100   | 100    |
| 139.00 | 17.70 | 25.65# |
| 279.00 | 35.40 | 38.75  |
| 0.00   | 0.00  | 0.00   |