
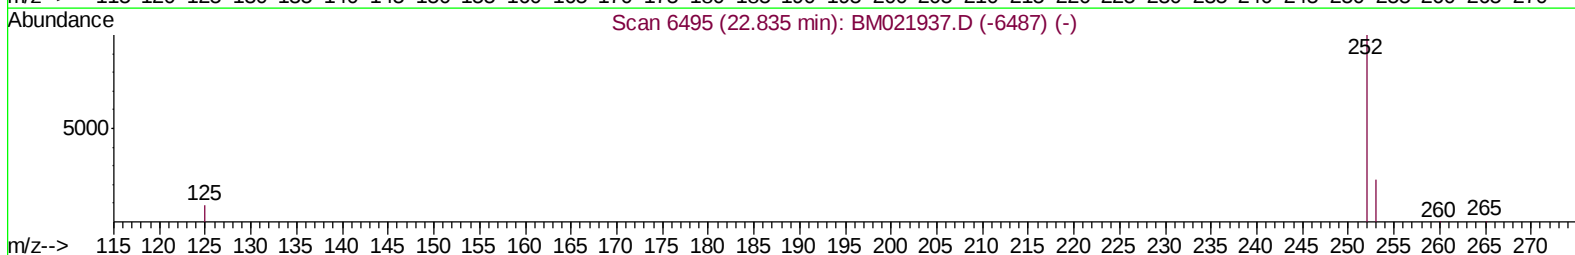
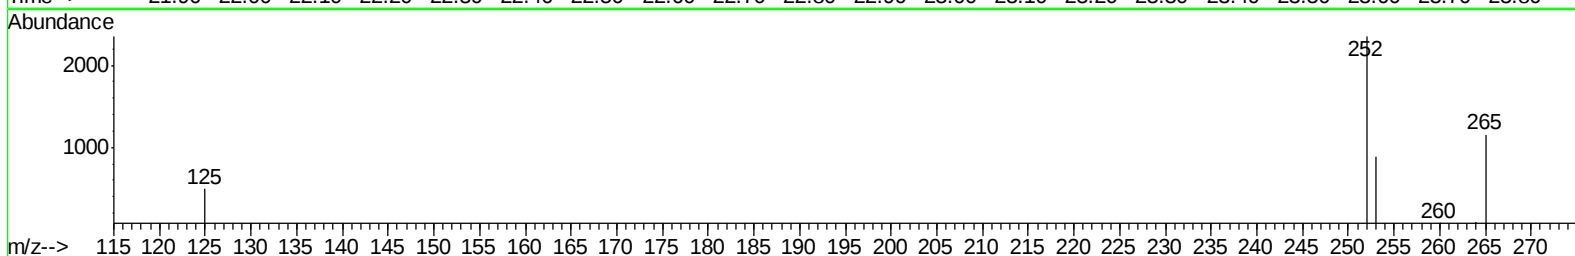


Data File : BM021941.D
Acq On : 08 Aug 2019 19:56
Operator : HP/JU
Sample : K4029-14DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 09 01:51:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

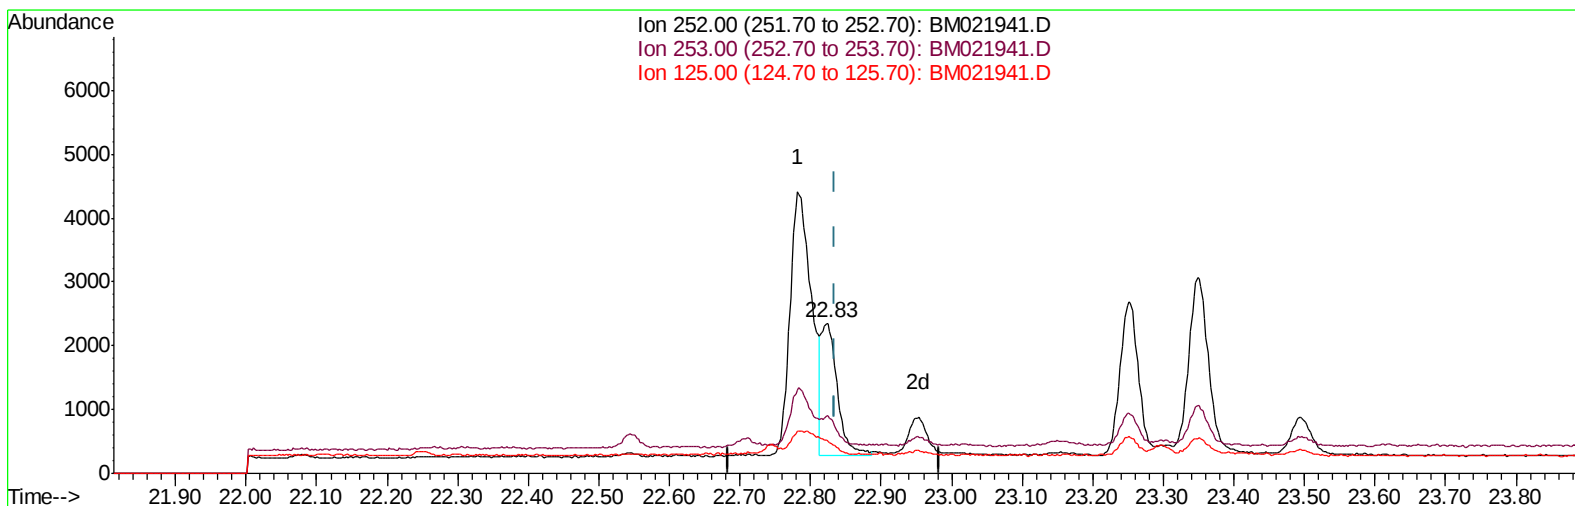

TIC: BM021941.D

(22) Benzo(k)fluoranthene

22.825min (-0.009) 0.17ng/ul m

response 3279

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	38.04
125.00	15.20	21.08#
0.00	0.00	0.00