

Data File : BM021914.D
Acq On : 08 Aug 2019 02:11
Operator : HP/JU
Sample : PB121841BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK49

Quant Time: Aug 08 04:43:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	878	0.40	ng/ul	0.00
2) Naphthalene-d8	10.40	136	3833	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	2161	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	391067	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	468141	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	1935	0.31	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.28	166	719	0.079	ng/ul#	Qvalue 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021914.D
Acq On : 08 Aug 2019 02:11
Operator : HP/JU
Sample : PB121841BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK49

Quant Time: Aug 08 04:43:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

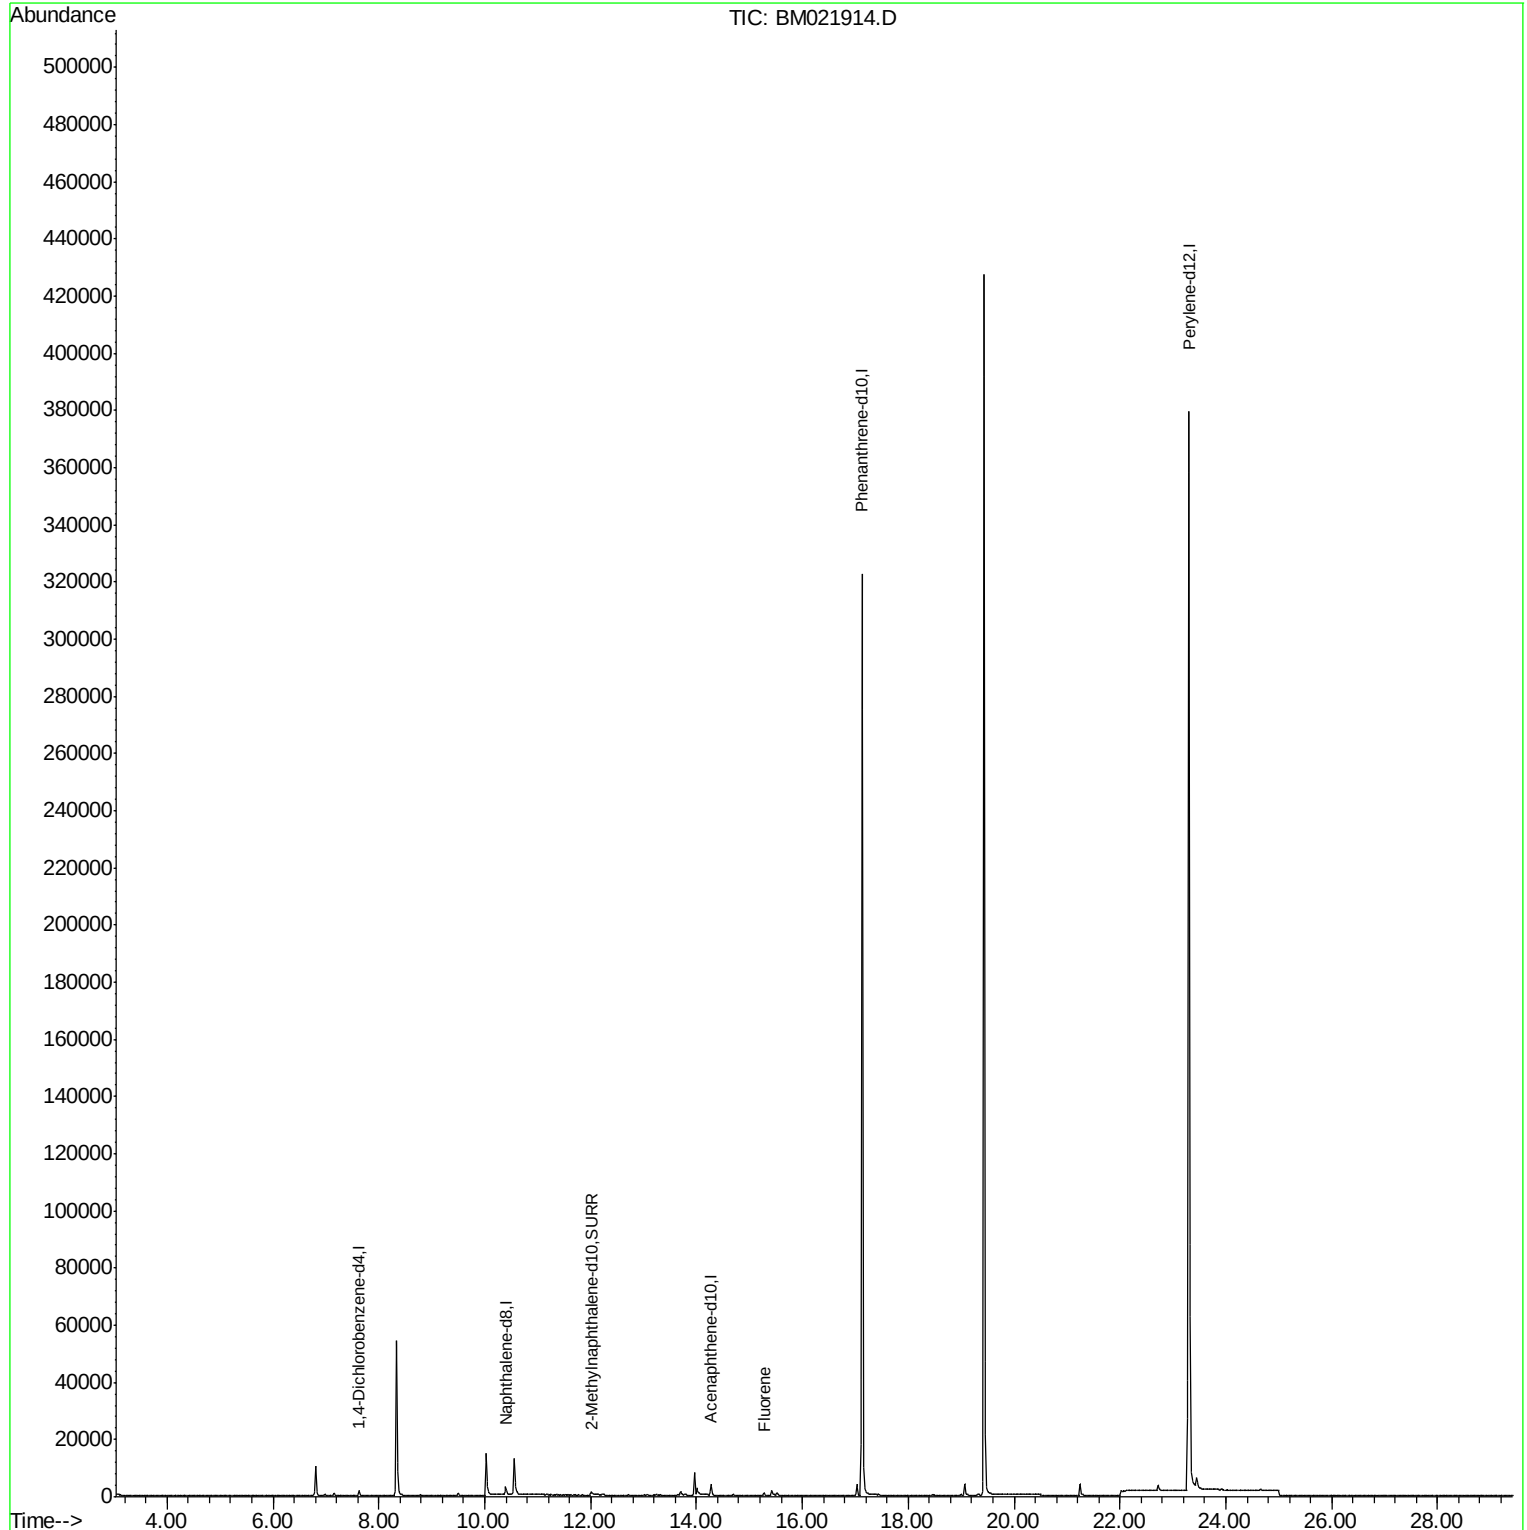

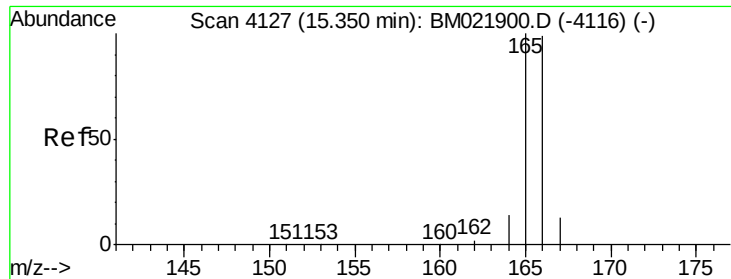

#9

Fluorene

Concen: 0.079 ng/ul

RT: 15.28 min Scan# 4107

Delta R.T. -0.07 min

Lab File: BM021914.D

Acq: 08 Aug 2019 02:11

Instrument :

BNA_M

ClientSampleId :

SBLK49


Tgt Ion:166 Resp: 719

Ion Ratio Lower Upper

166 100

165 14.7 81.4 122.0#

167 37.9 13.7 20.5#

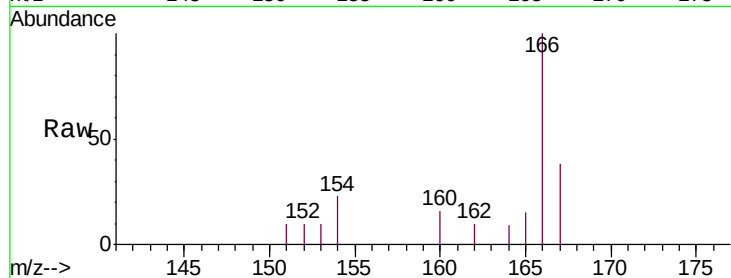

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

