

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Not Reviewed)

Data File : BM021919.D
Acq On : 08 Aug 2019 05:49
Operator : HP/JU
Sample : K4028-21
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENW4

Quant Time: Aug 08 06:57:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 06:54:24 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	917	0.40	ng/ul	0.00
2) Naphthalene-d8	10.40	136	4054	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	2205	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	206006	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	255163	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	993	0.15	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
7) Acenaphthylene	14.00	152	341	0.033	ng/ul#	Qvalue 66




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021919.D
Acq On : 08 Aug 2019 05:49
Operator : HP/JU
Sample : K4028-21
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENW4

Quant Time: Aug 08 06:57:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 06:54:24 2019
Response via : Initial Calibration

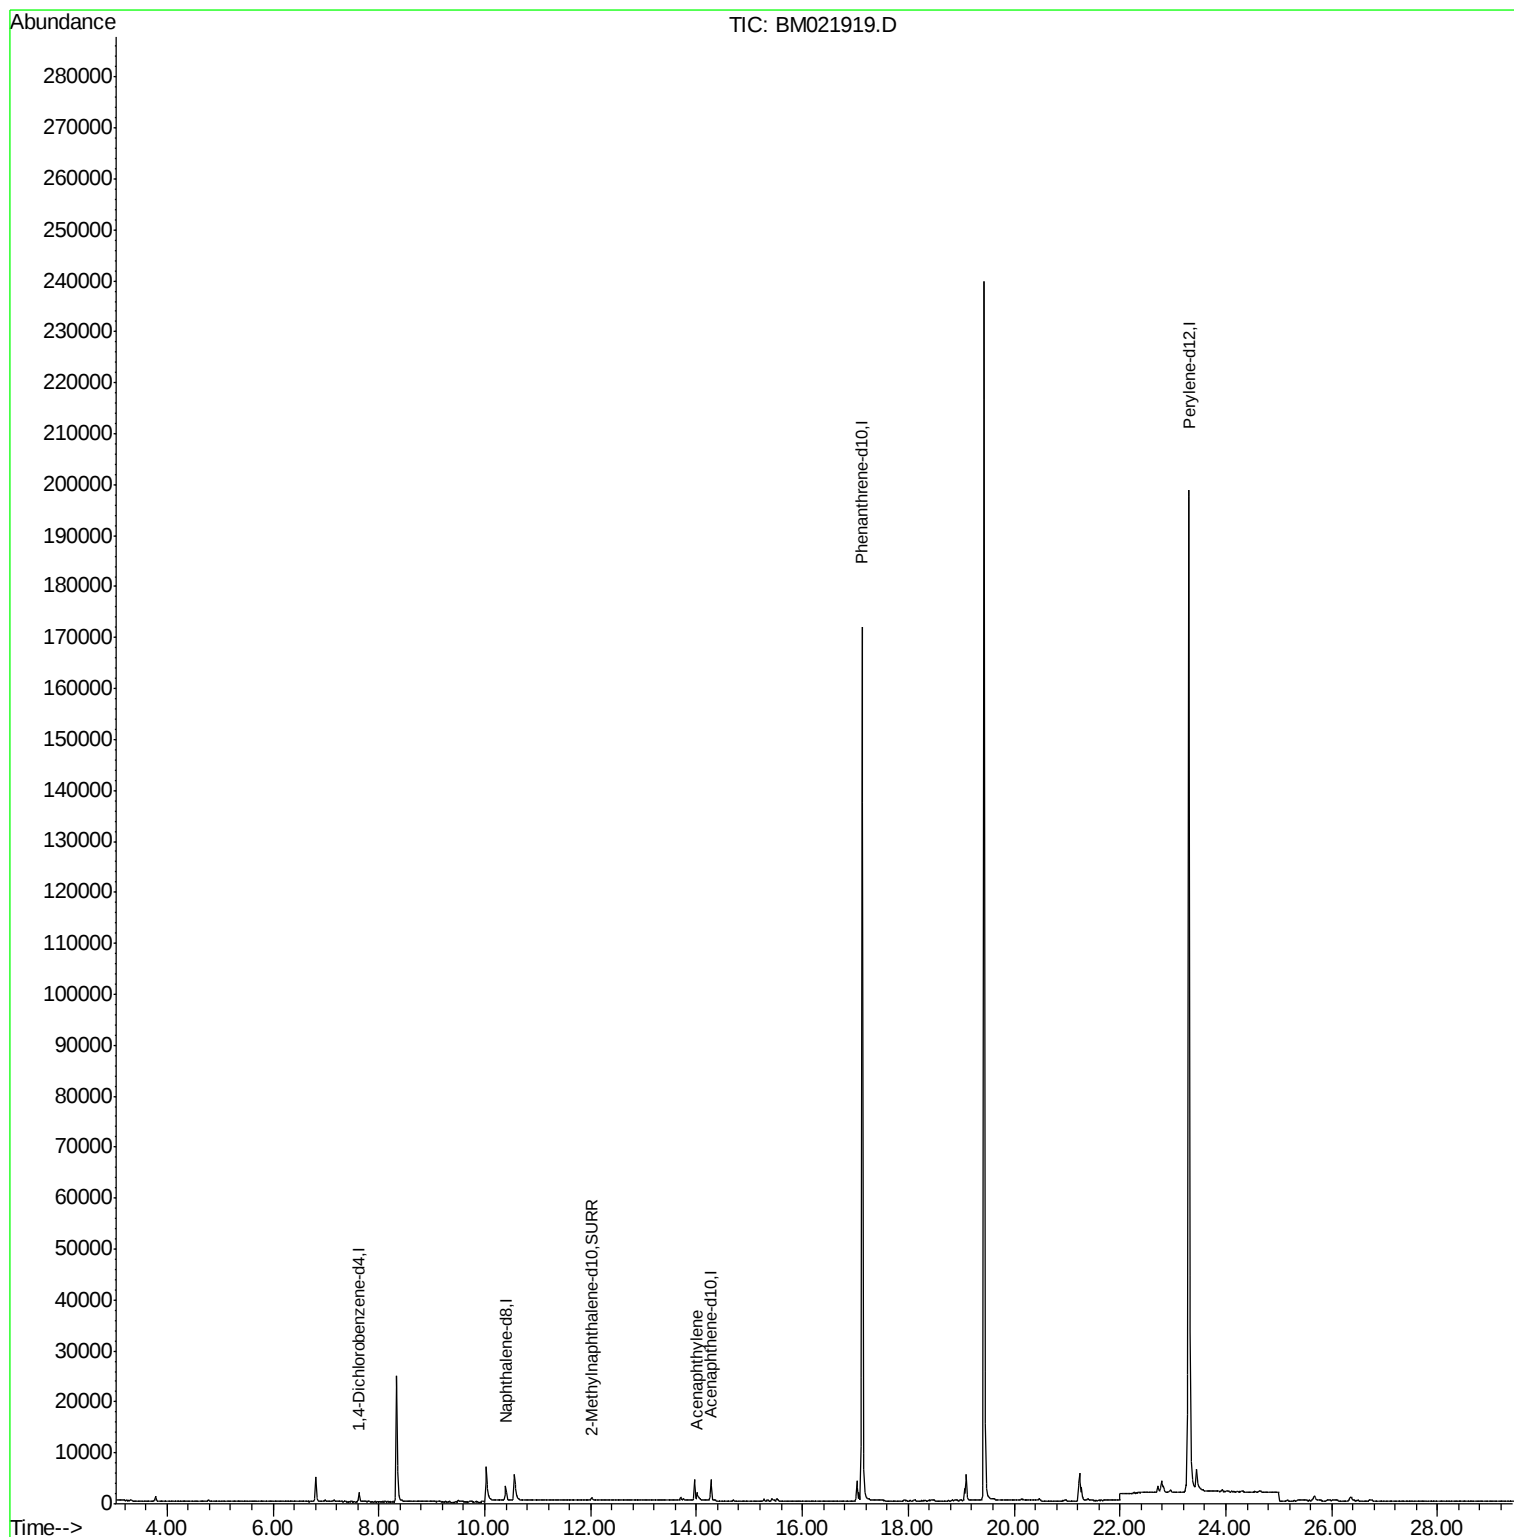

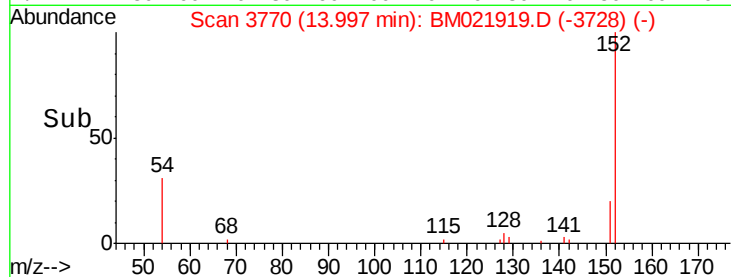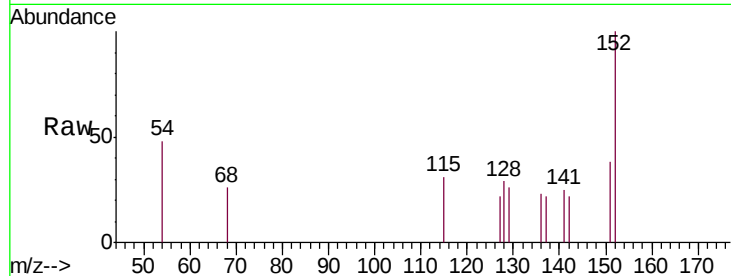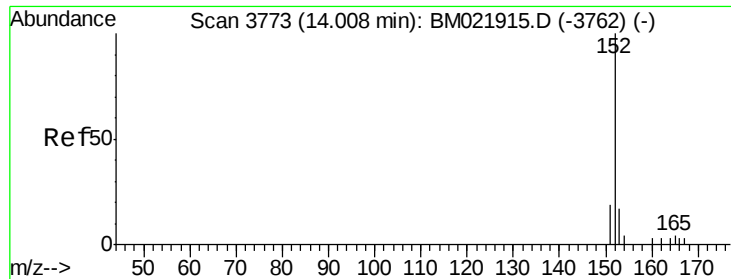

#7

Acenaphthylene

Concen: 0.033 ng/ul

RT: 14.00 min Scan# 3770

Delta R.T. -0.01 min

Lab File: BM021919.D

Acq: 08 Aug 2019 05:49

Instrument :

BNA_M

ClientSampleId :

BENW4

Tgt Ion:152 Resp: 341

Ion Ratio Lower Upper

152 100

151 38.2 18.3 27.5#

153 0.0 12.8 19.2#

