

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Not Reviewed)

Data File : BM021945.D
Acq On : 08 Aug 2019 22:23
Operator : HP/JU
Sample : K4116-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLE0

Quant Time: Aug 09 01:33:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	730	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	3131	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	1718	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	272731	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	324089	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	1733	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.27	166	506	0.069	ng/ul#	Qvalue 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021945.D
Acq On : 08 Aug 2019 22:23
Operator : HP/JU
Sample : K4116-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLE0

Quant Time: Aug 09 01:33:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

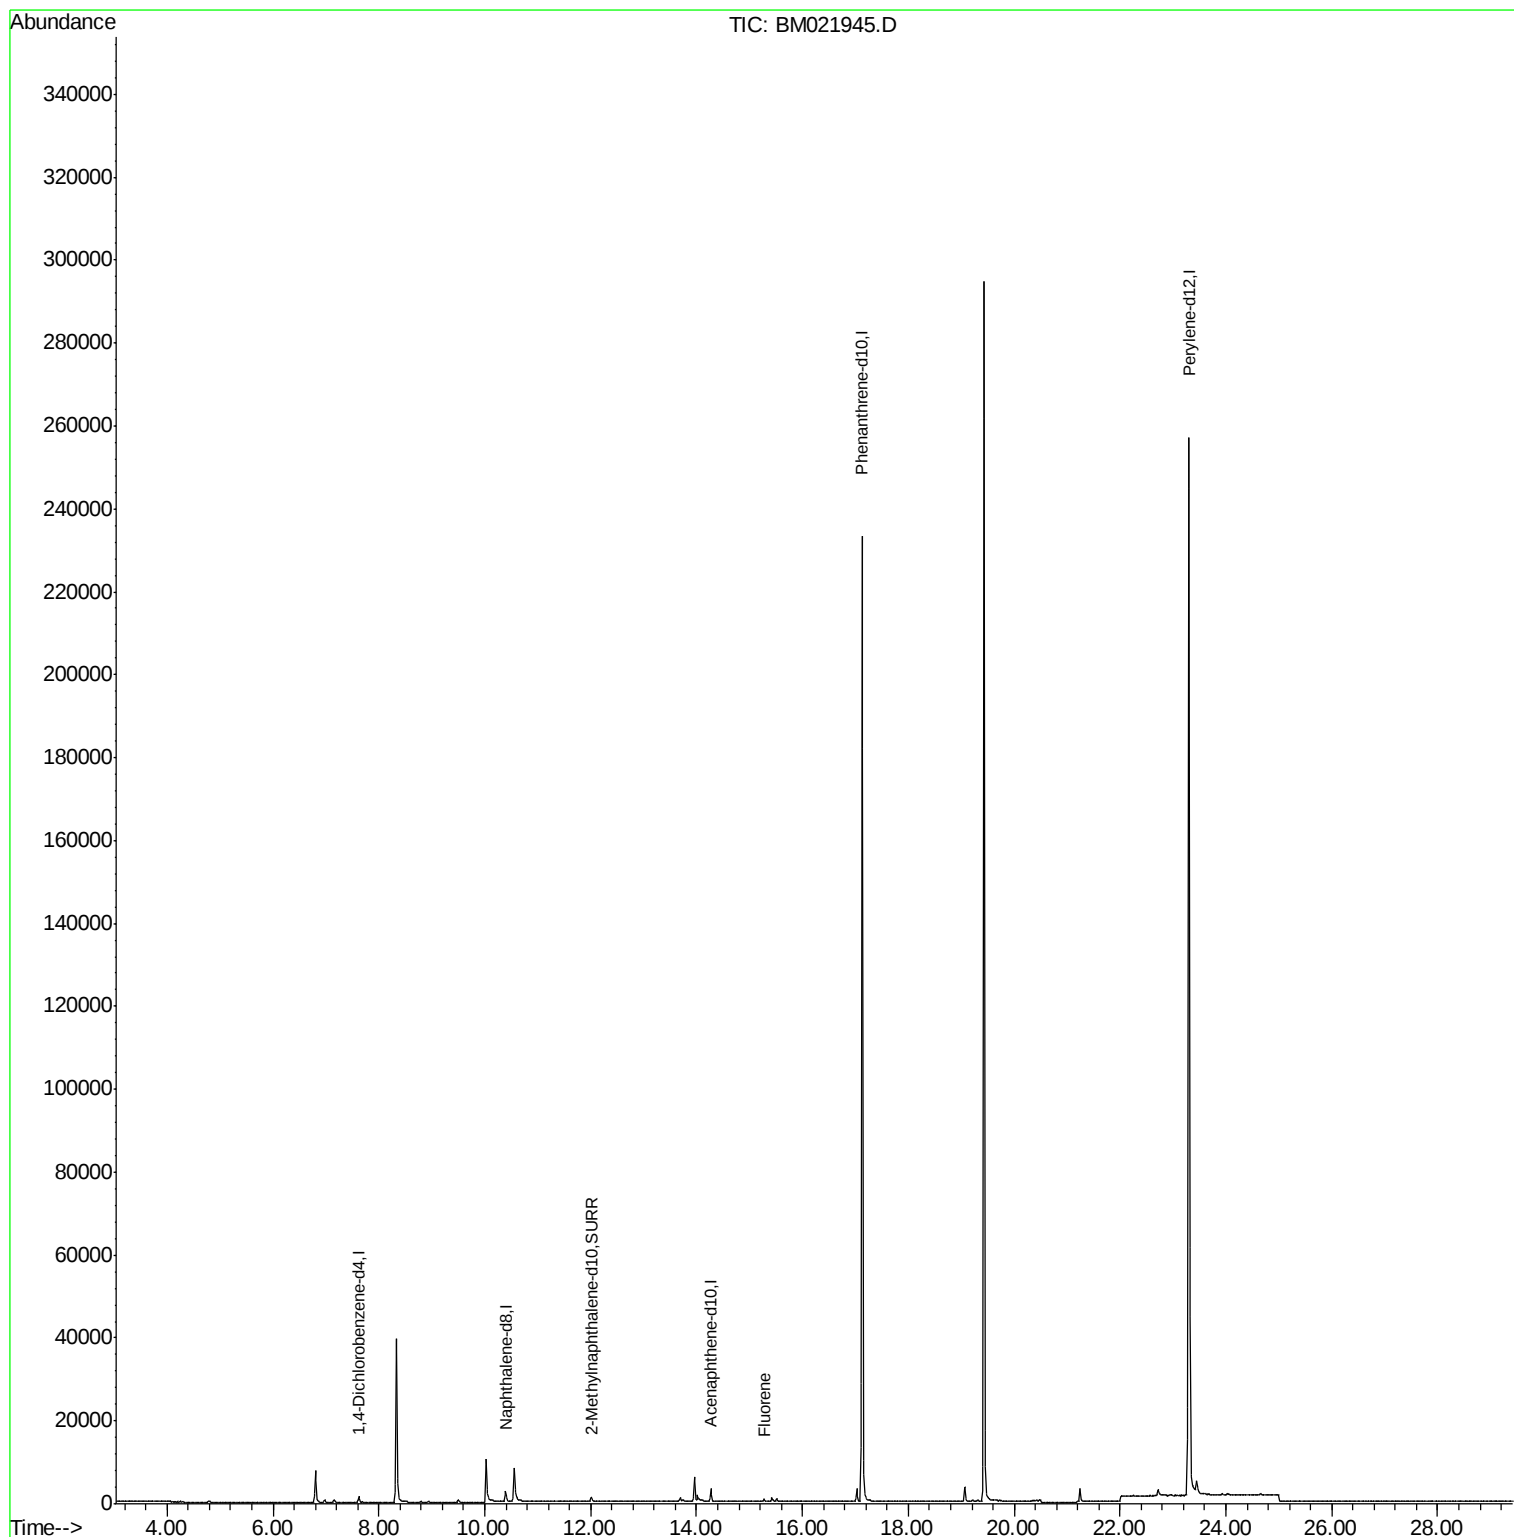

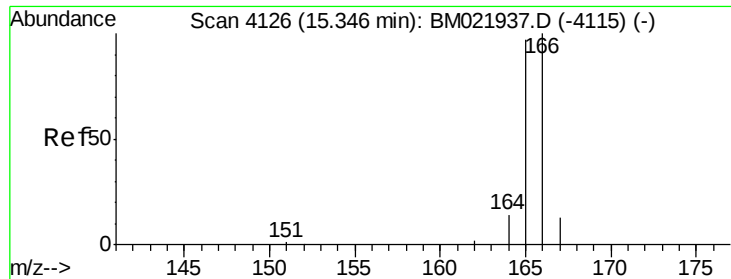

#9

Fluorene

Concen: 0.069 ng/ul

RT: 15.27 min Scan# 4106

Delta R.T. -0.07 min

Lab File: BM021945.D

Acq: 08 Aug 2019 22:23

Instrument :

BNA_M

ClientSampleId :

JLLE0



Tgt Ion:166 Resp: 506

Ion Ratio Lower Upper

166 100

165 18.9 81.4 122.0#

167 40.5 13.7 20.5#

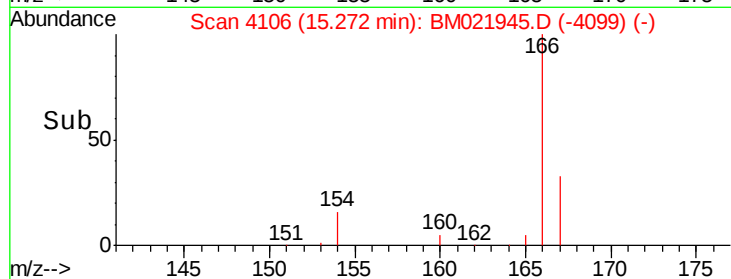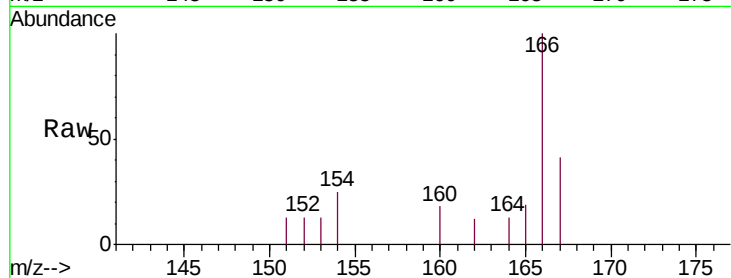

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

500

400

300

200

100

0

15.27

15.25

15.30

Time-->