

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080719\
 Data File : BM021959.D
 Acq On : 09 Aug 2019 08:05
 Operator : HP/JU
 Sample : K4116-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 09 09:21:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	1037	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	4310	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	2356	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.12	188	237815	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	306444	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	1488	0.21	ng/ul	-0.02
14) Fluoranthene-d10	19.17	212	285	0.00	ng/ul	0.09
Target Compounds						
7) Acenaphthylene	13.99	152	327	0.030	ng/ul#	Ovalue 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080719\
Data File : BM021959.D
Acq On : 09 Aug 2019 08:05
Operator : HP/JU
Sample : K4116-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 09 09:21:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

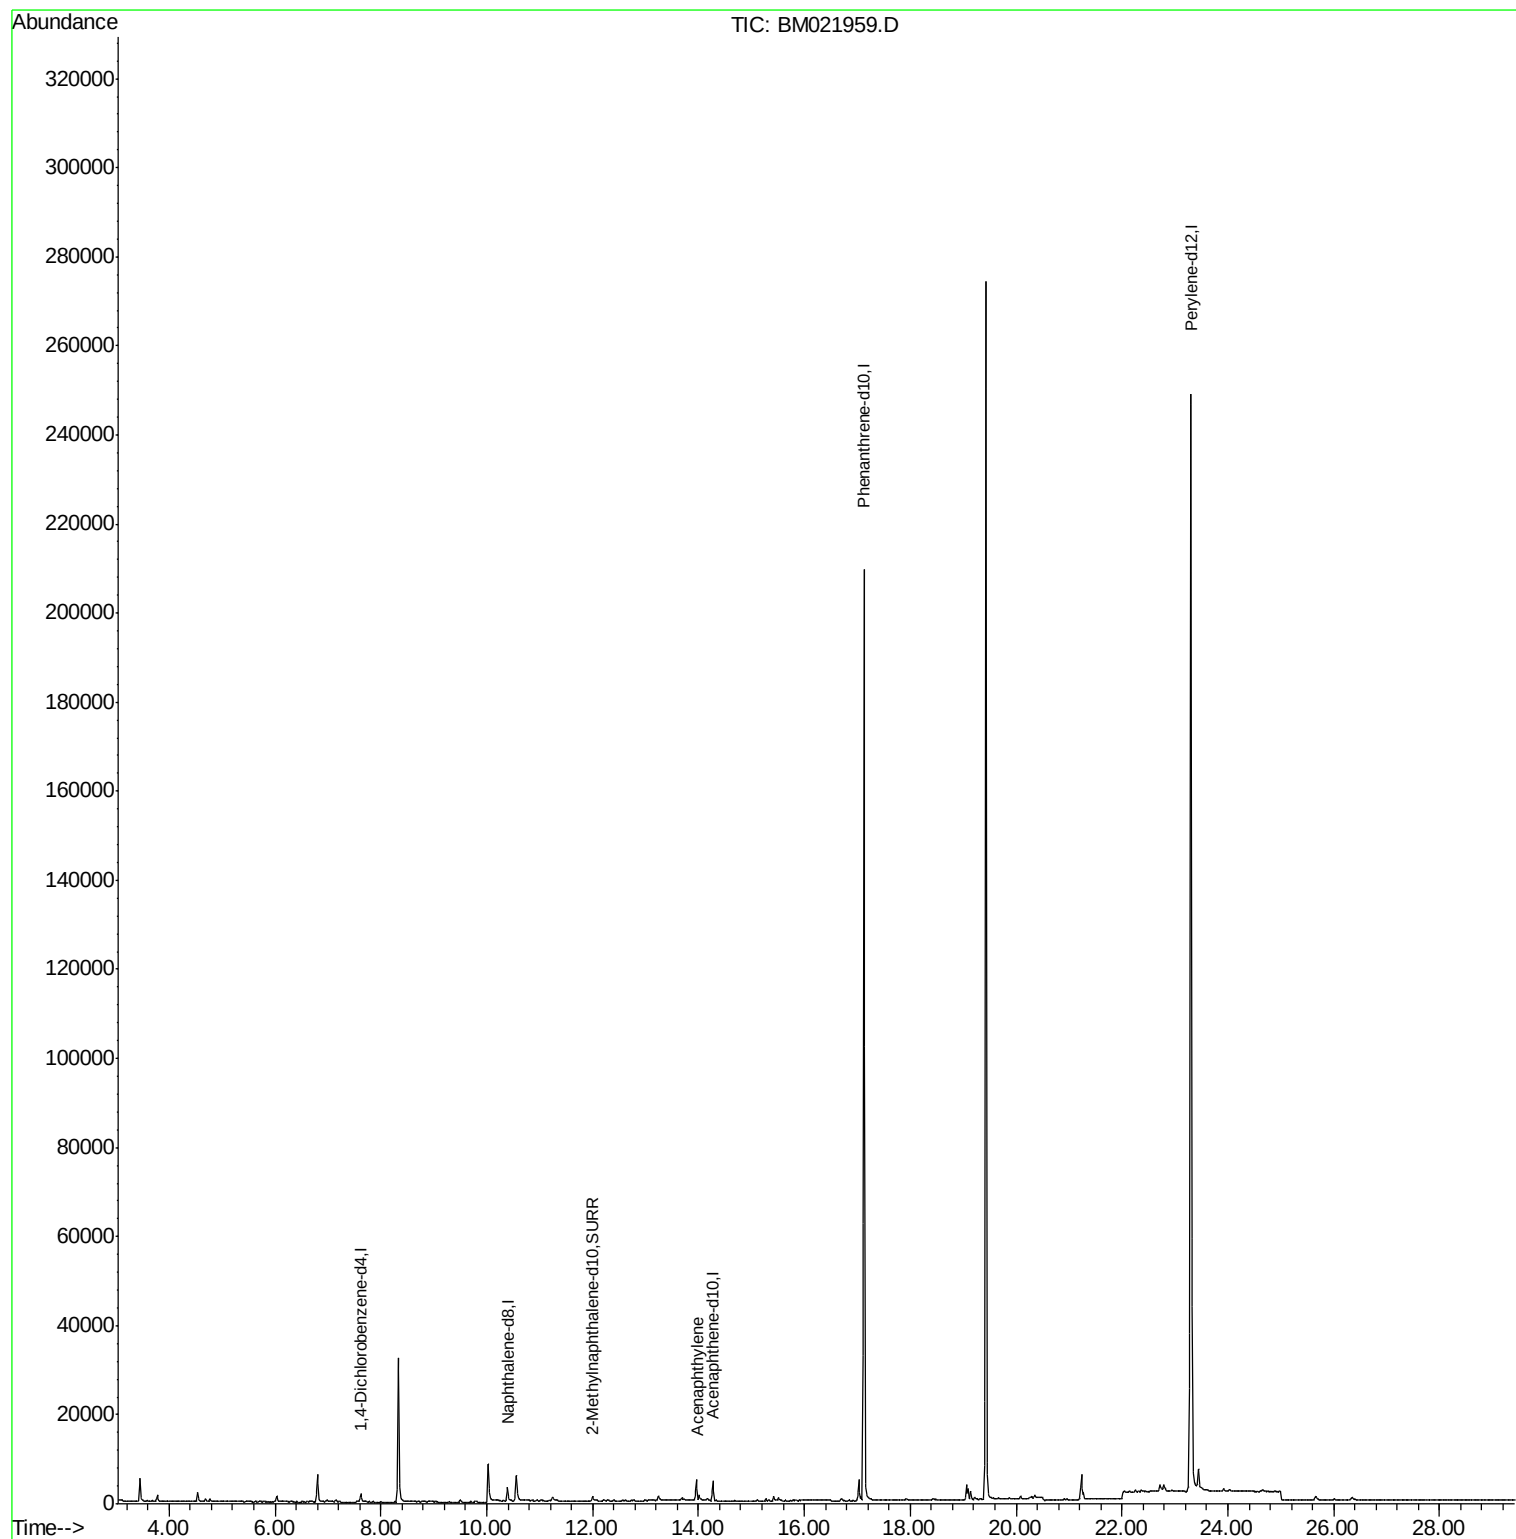

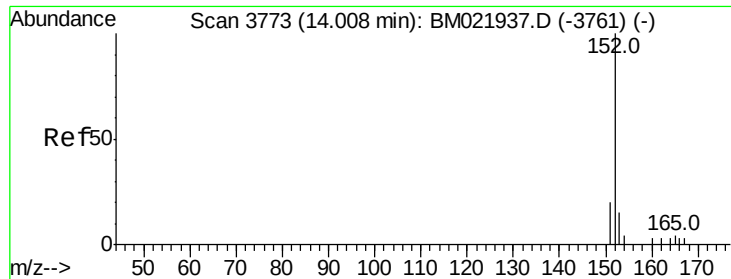

#7

Acenaphthylene

Concen: 0.030 ng/ul

RT: 13.99 min Scan# 3769

Delta R.T. -0.02 min

Lab File: BM021959.D

Acq: 09 Aug 2019 08:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:152 Resp: 327

Ion Ratio Lower Upper

152 100

151 42.7 18.3 27.5#

153 0.0 12.8 19.2#

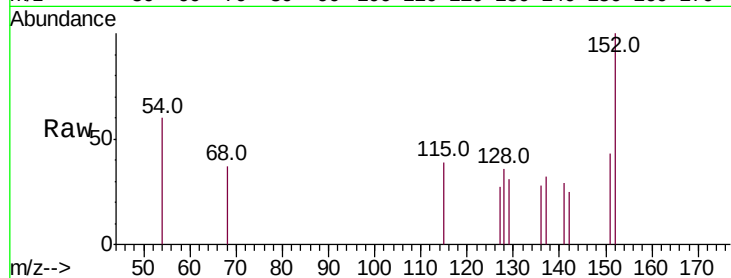

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

