

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (QT Reviewed)


Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:37:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

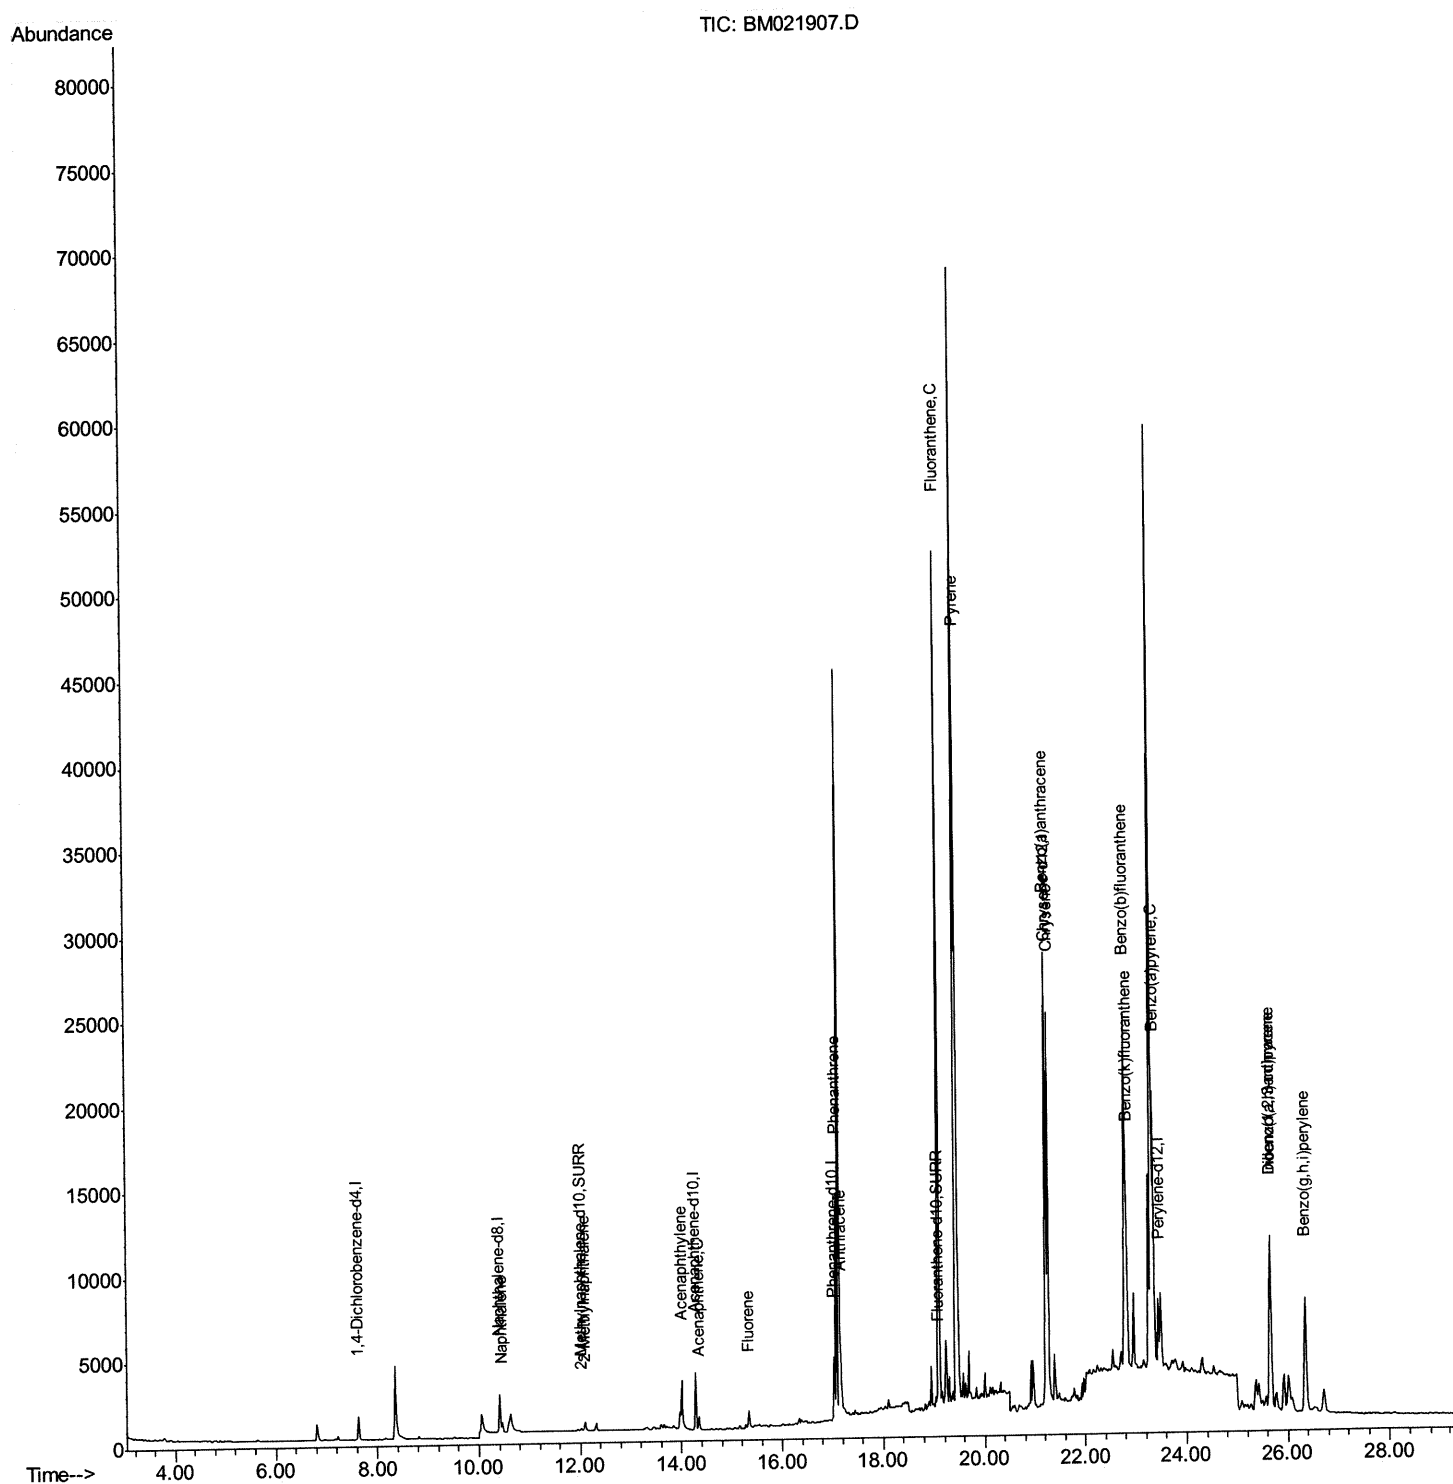

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)



Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 04:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

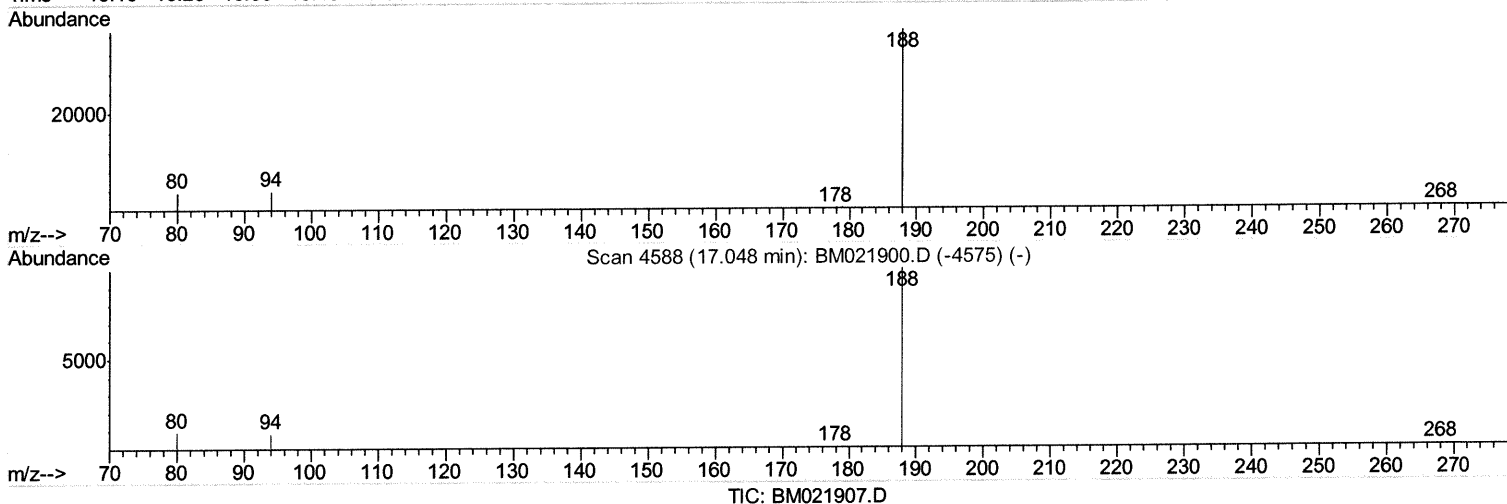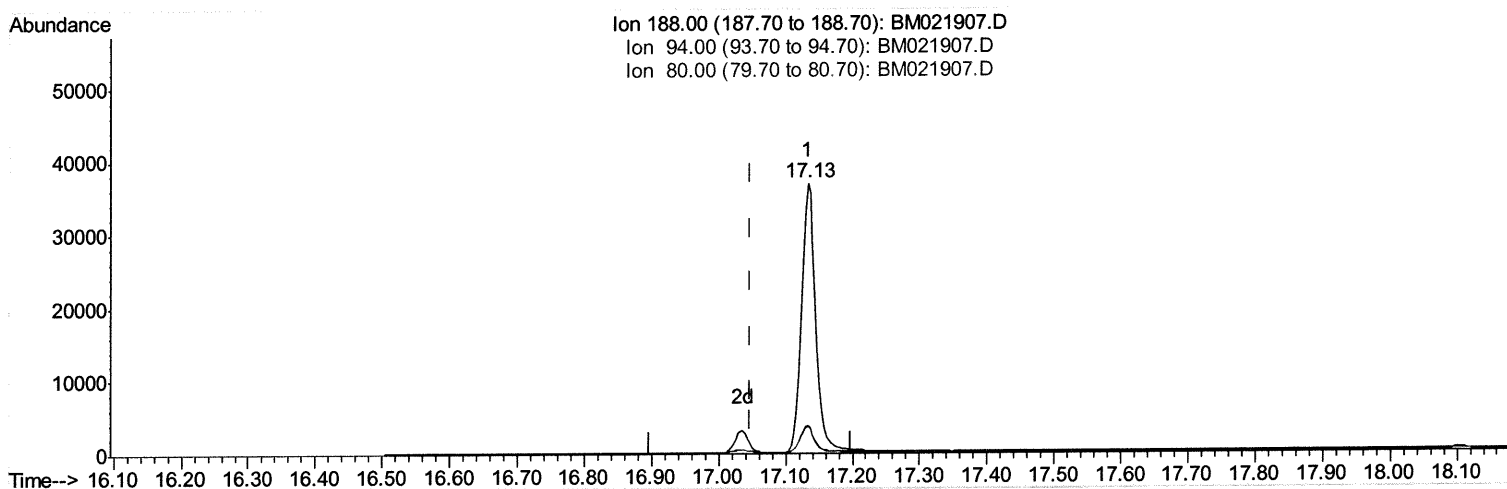

(10) Phenanthrene-d10 (I)

17.133min (+0.085) 0.40ng/ul

response 54284

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.41
80.00	11.40	9.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)



Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 04:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

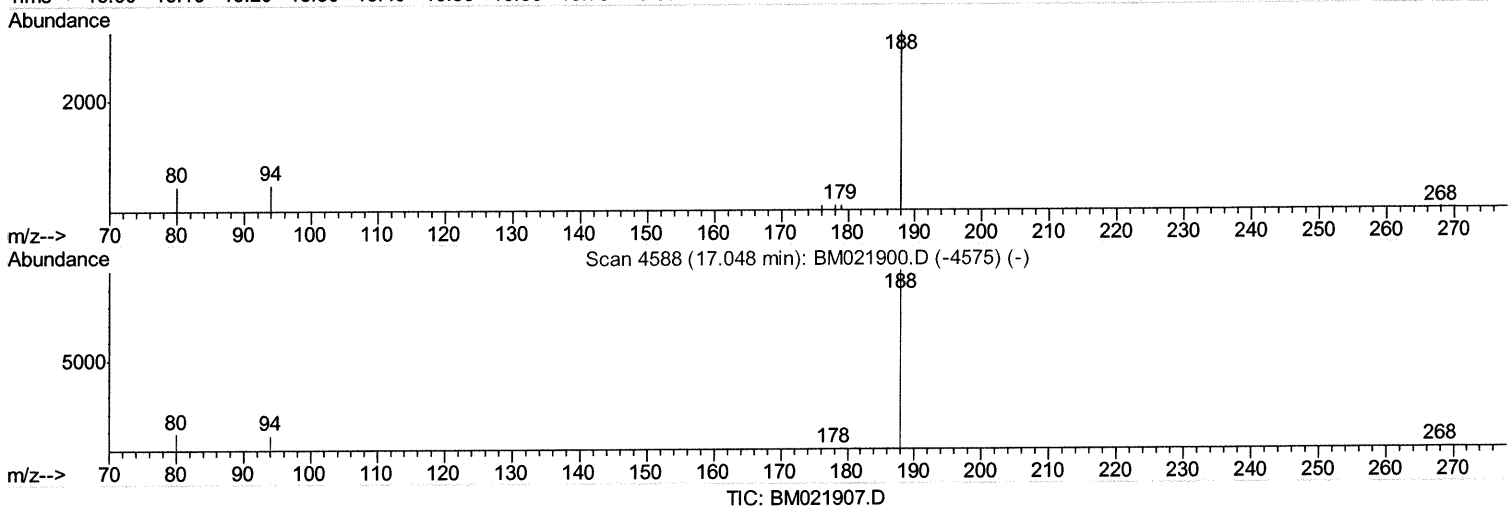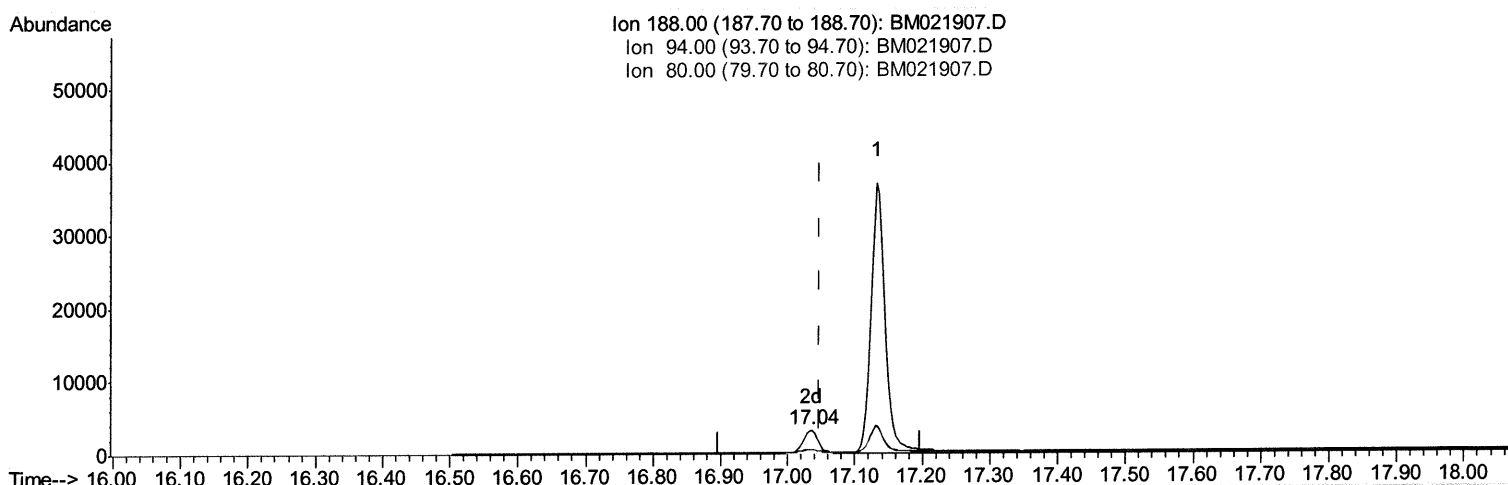

(10) Phenanthrene-d10 (I)

17.036min (-0.012) 0.40ng/ul m

JU
08/08/19

response 4820

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	15.82#
80.00	11.40	15.10#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

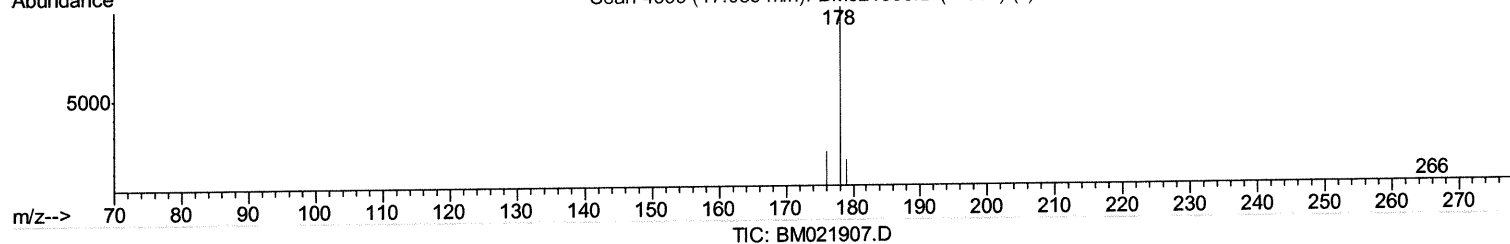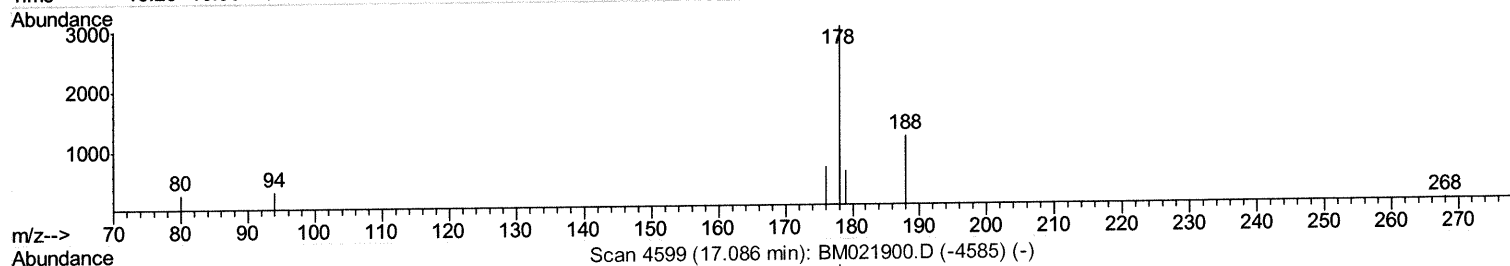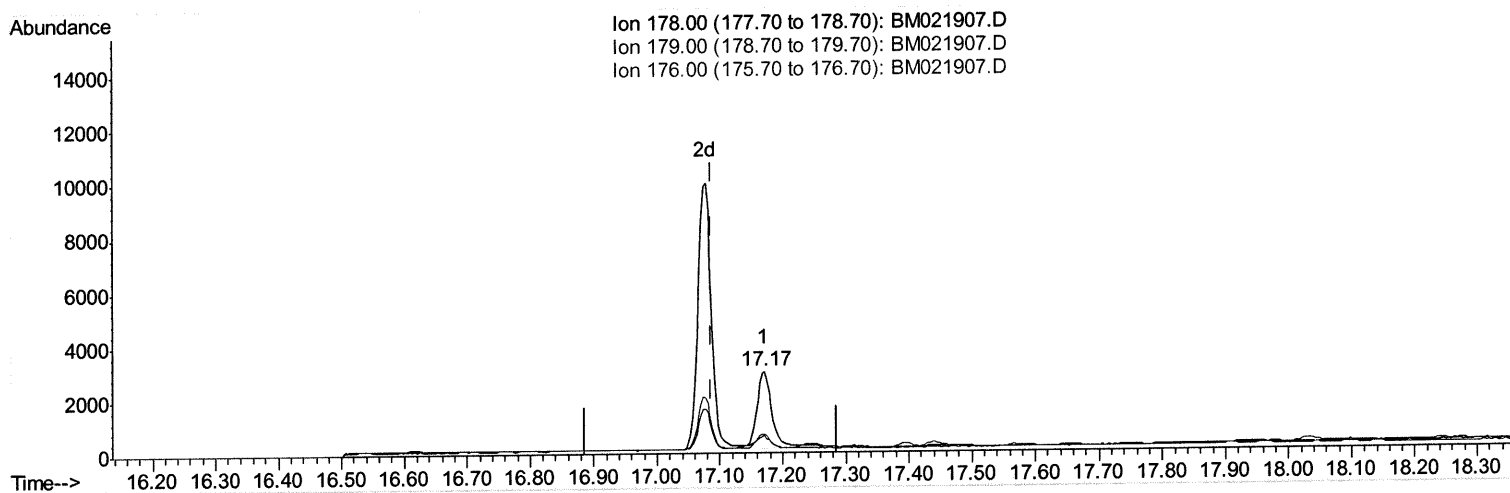

(12) Phenanthrene

17.171min (+0.085) 0.36ng/ul

response 5038

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	20.49
176.00	21.00	22.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)



Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

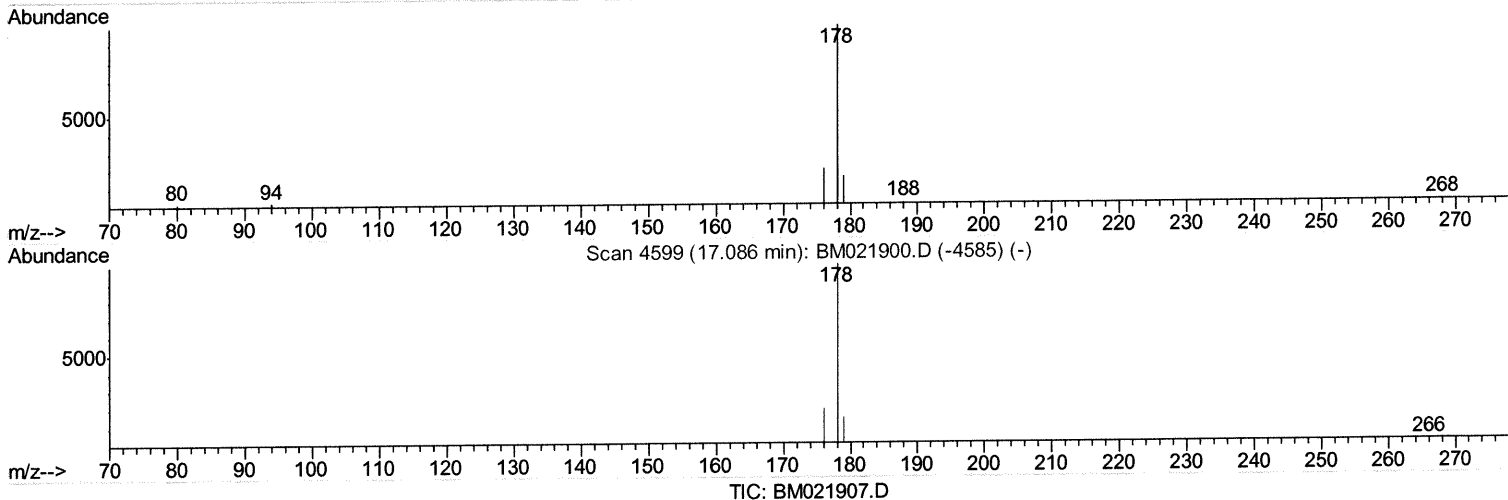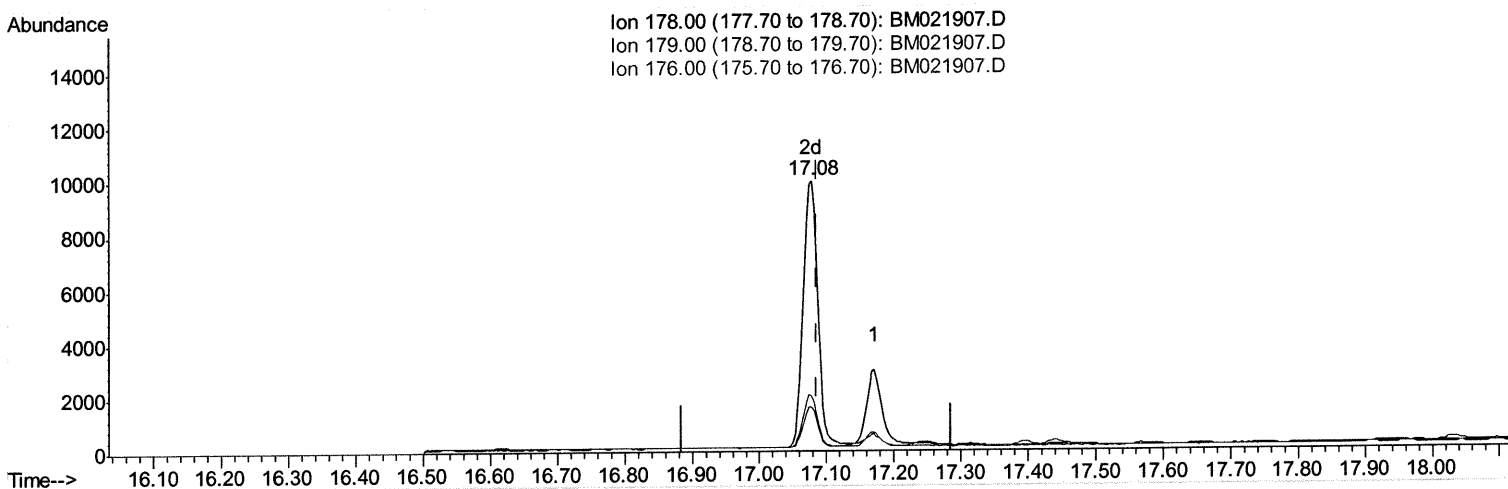

(12) Phenanthrene

17.077min (-0.009) 1.06ng/ul m

JU
08/08/19

response 14816

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	16.47
176.00	21.00	20.48
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

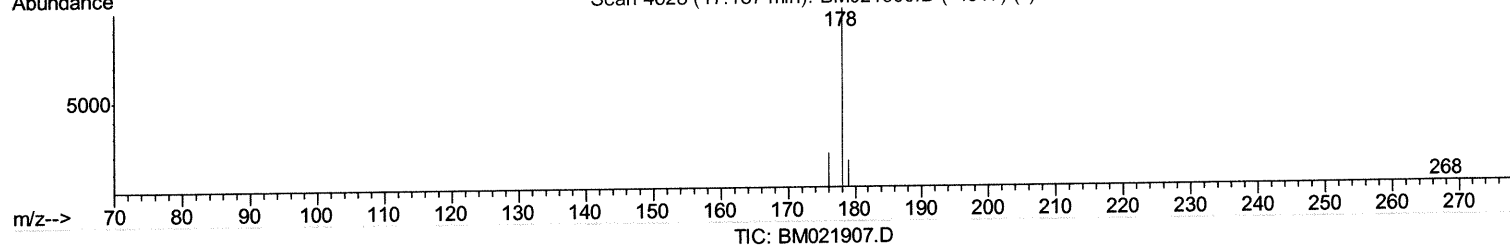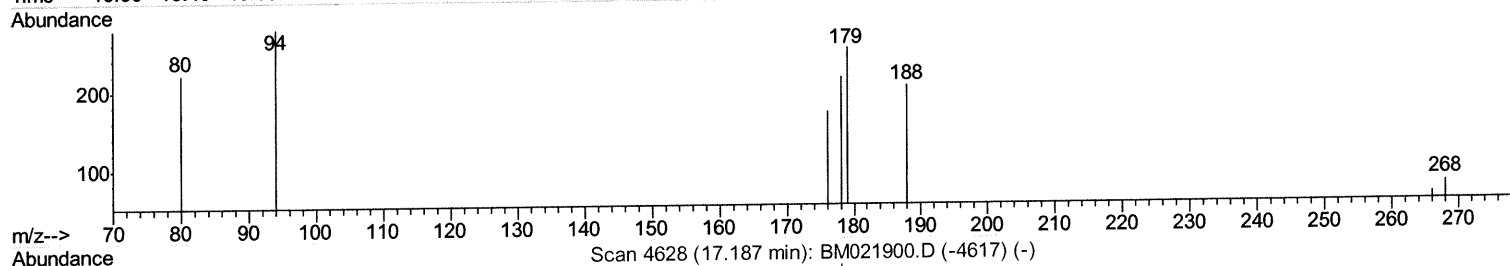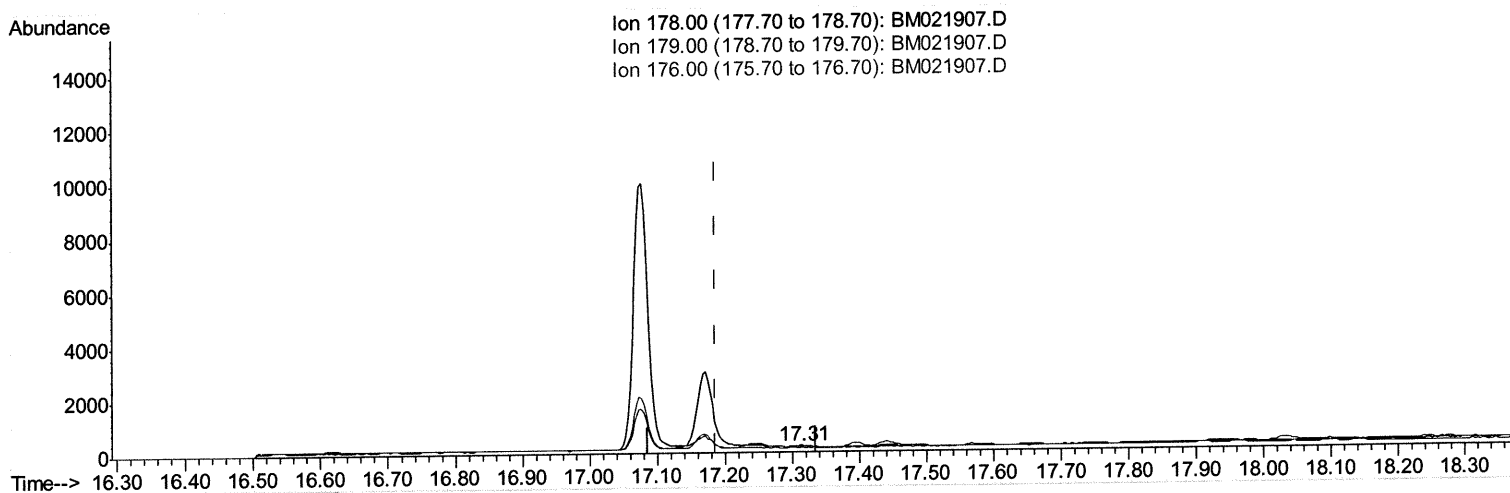

(13) Anthracene

17.313min (+0.127) 0.01ng/ul

response 102

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	117.84#
176.00	20.80	79.34#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

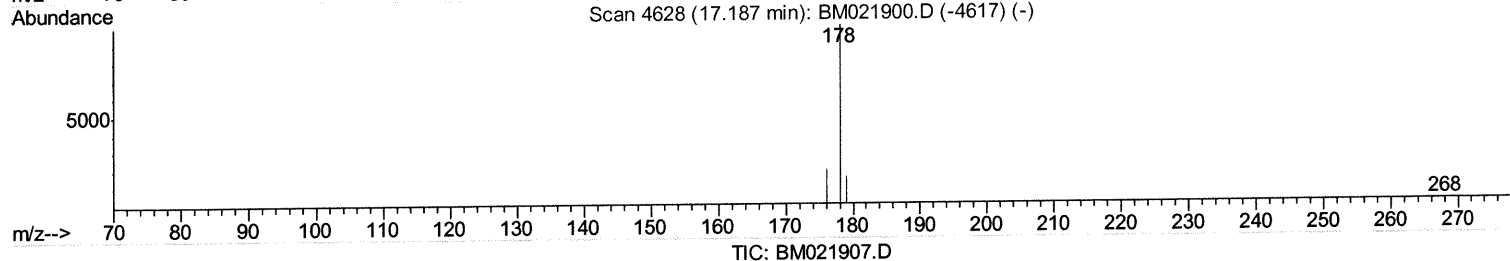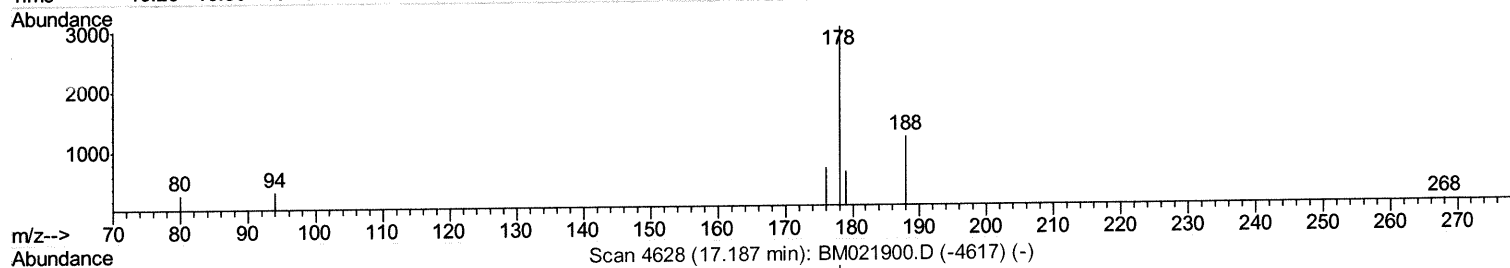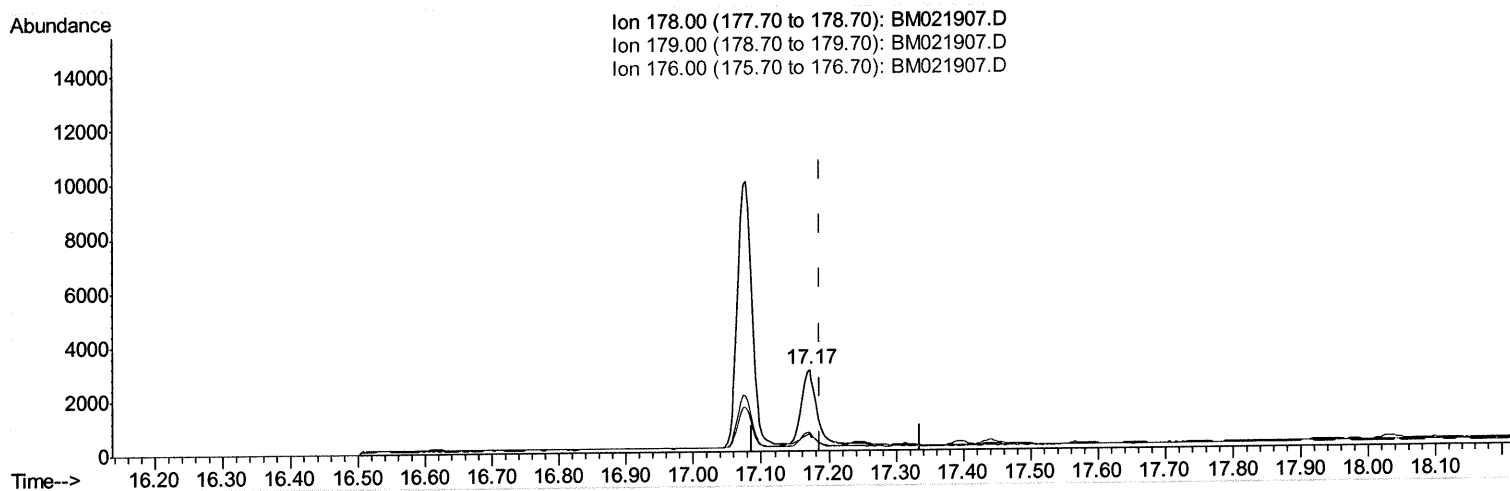

(13) Anthracene

17.171min (-0.016) 0.36ng/ul m

JU
08/08/19

response 4283

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	20.49
176.00	20.80	22.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

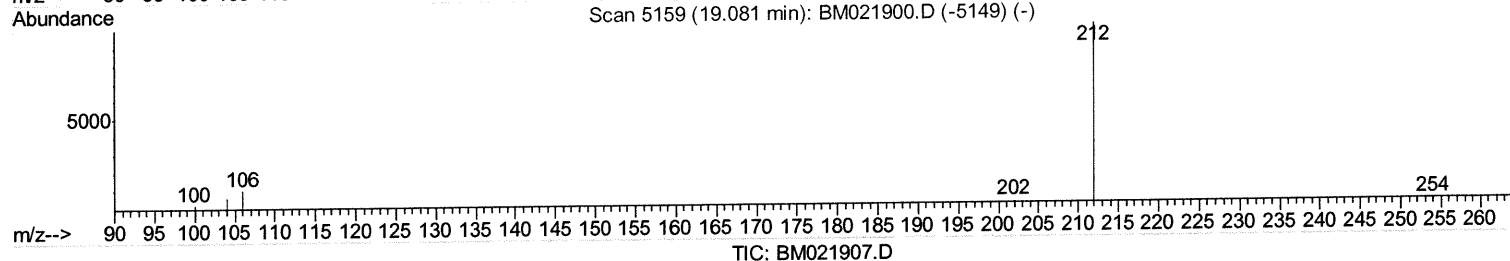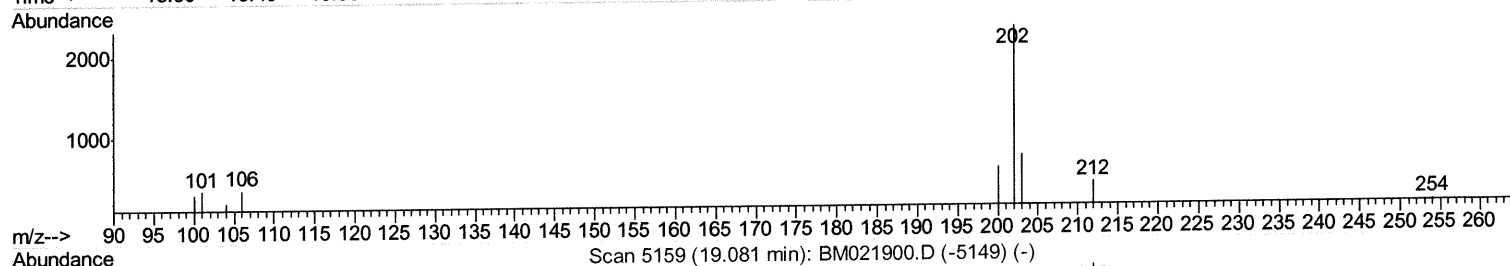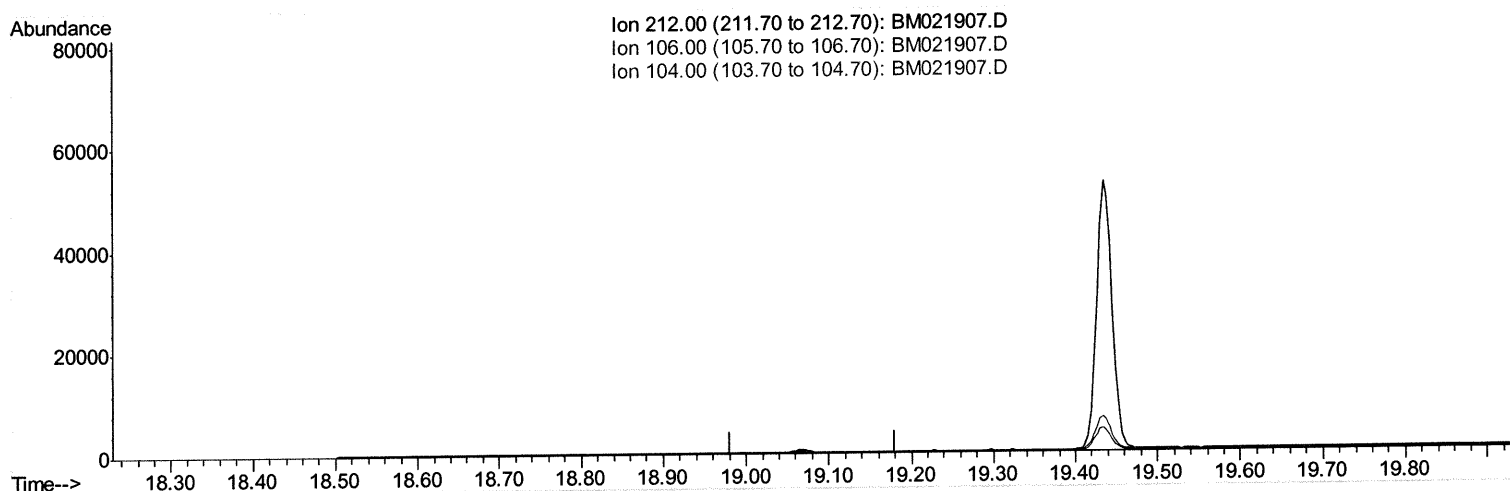

(14) Fluoranthene-d10 (SURR)

19.081min (-19.081) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

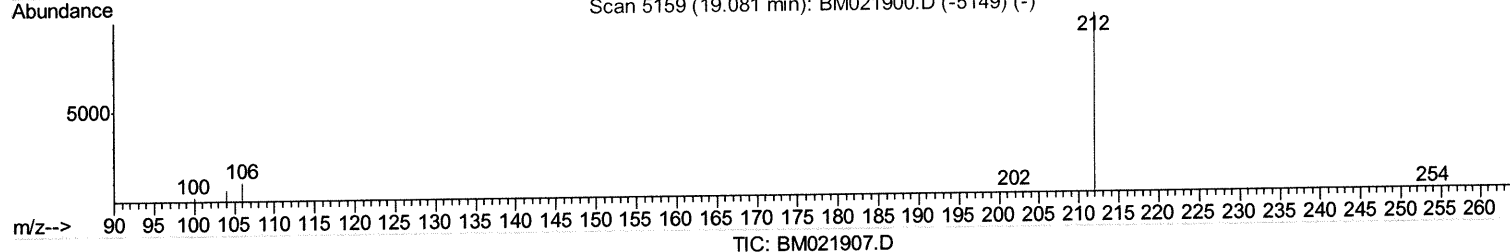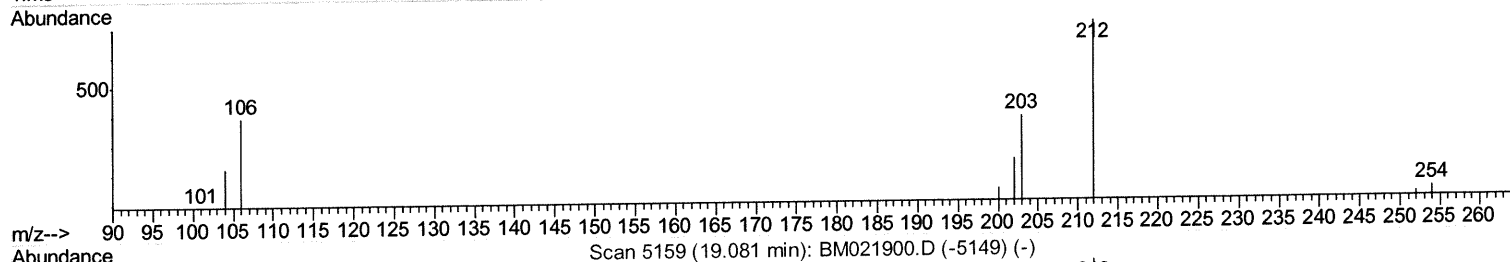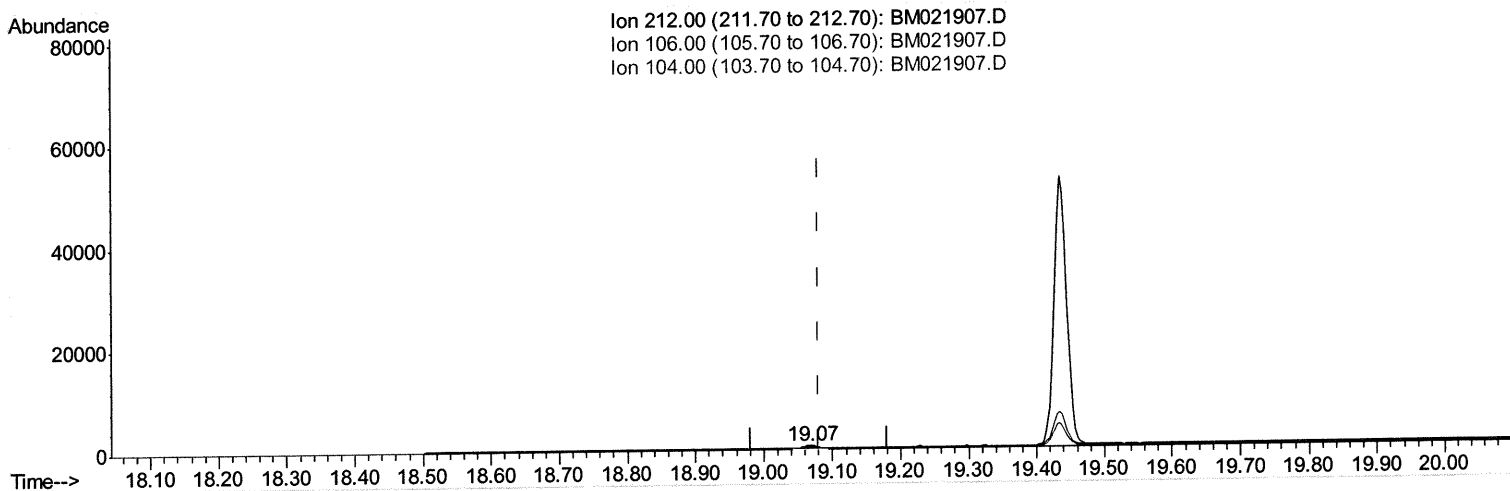

(14) Fluoranthene-d10 (SURR)

19.068min (-0.013) 0.05ng/ul m

JU
08/08/19

response 852

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

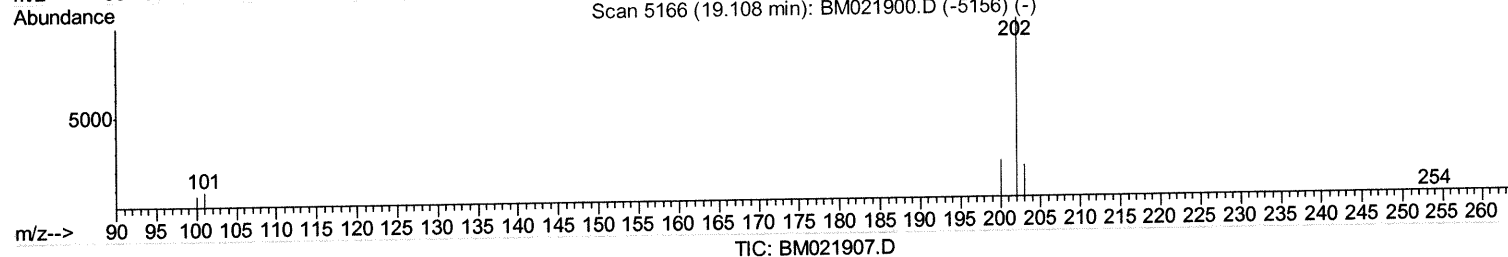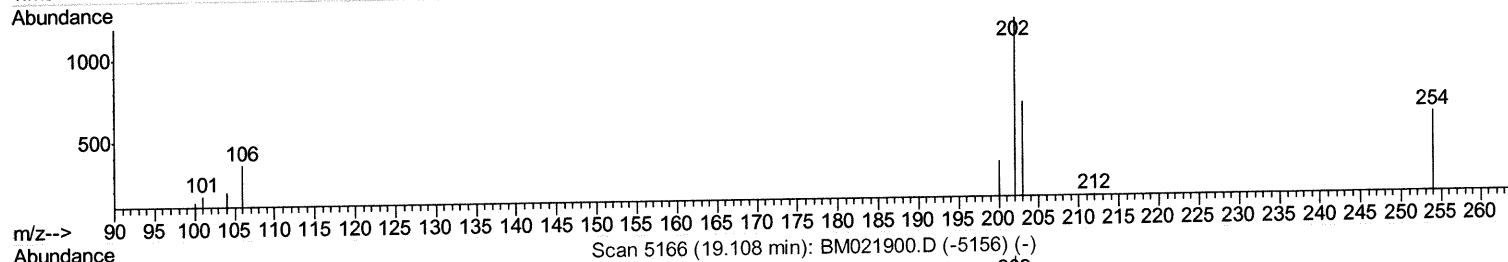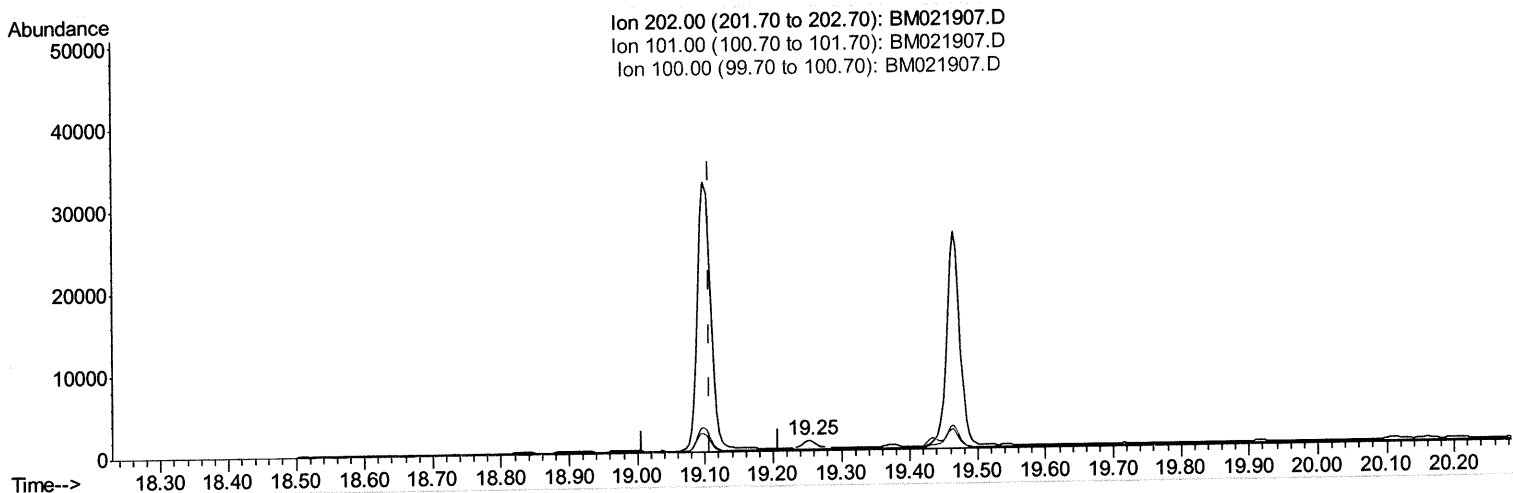

(15) Fluoranthene (C)

19.255min (+0.147) 0.06ng/ul

response 1198

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	14.12
100.00	8.10	11.11
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)



Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

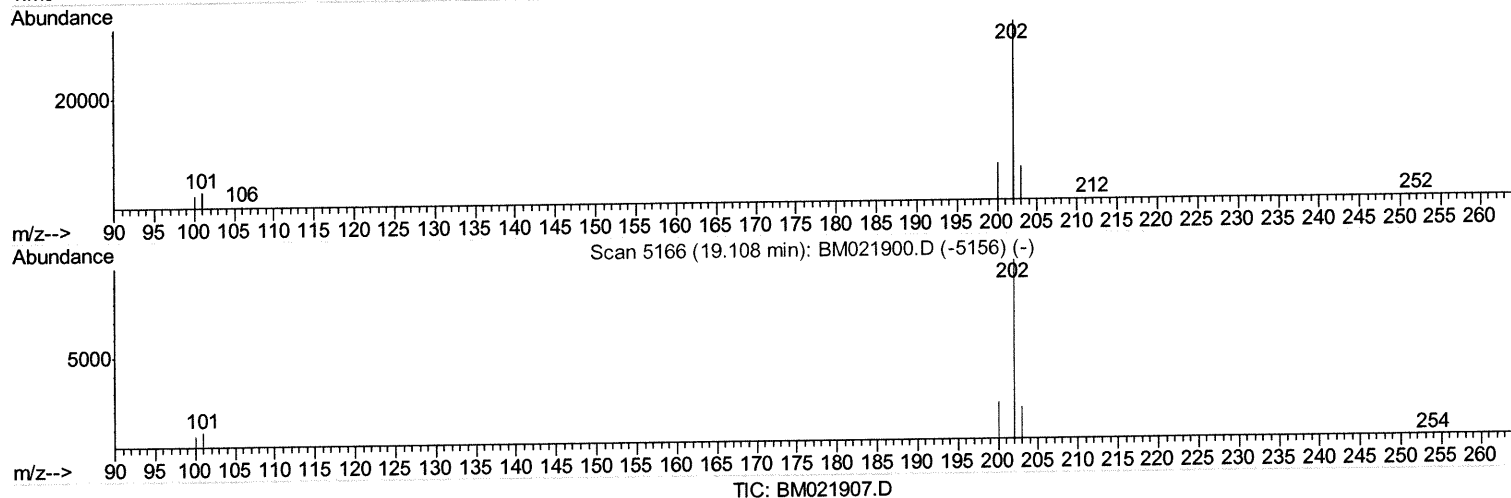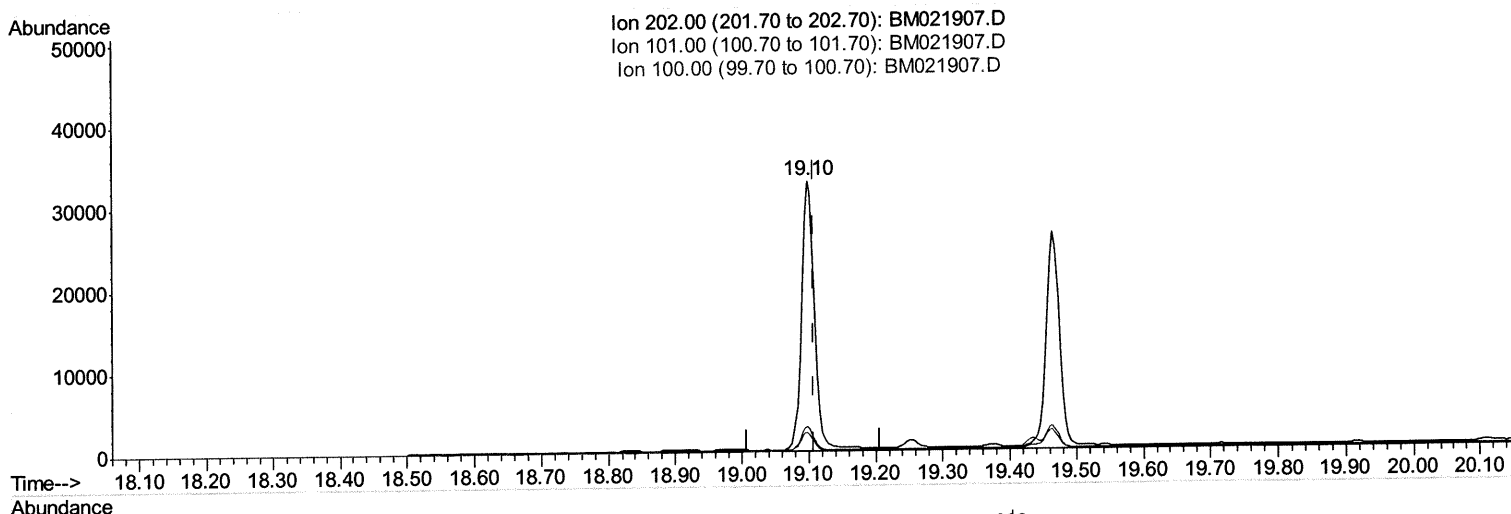

(15) Fluoranthene (C)

19.098min (-0.009) 2.33ng/ul m

JU
08/08/19

response 43703

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	9.16
100.00	8.10	7.06
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

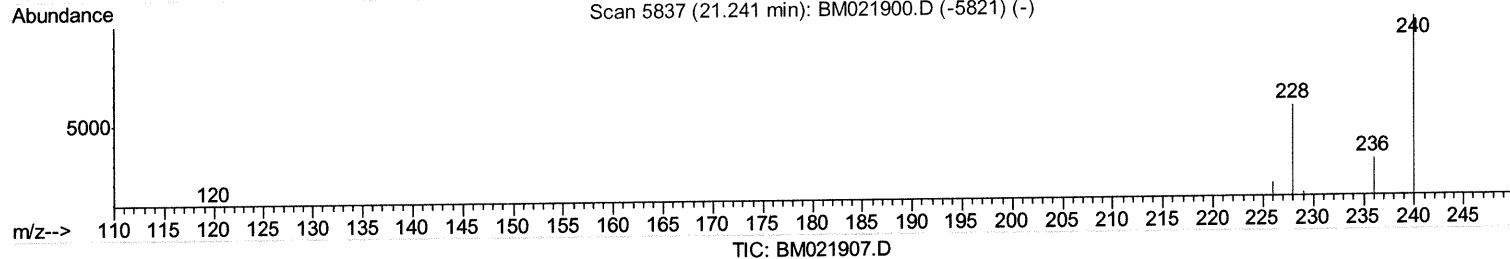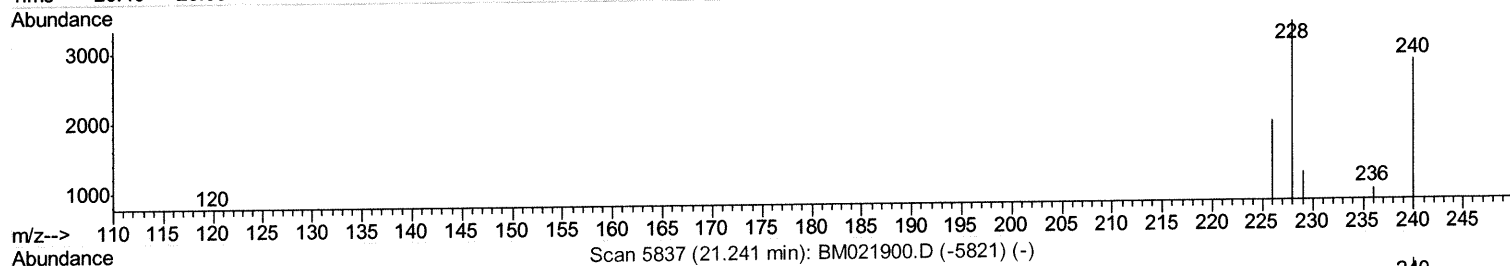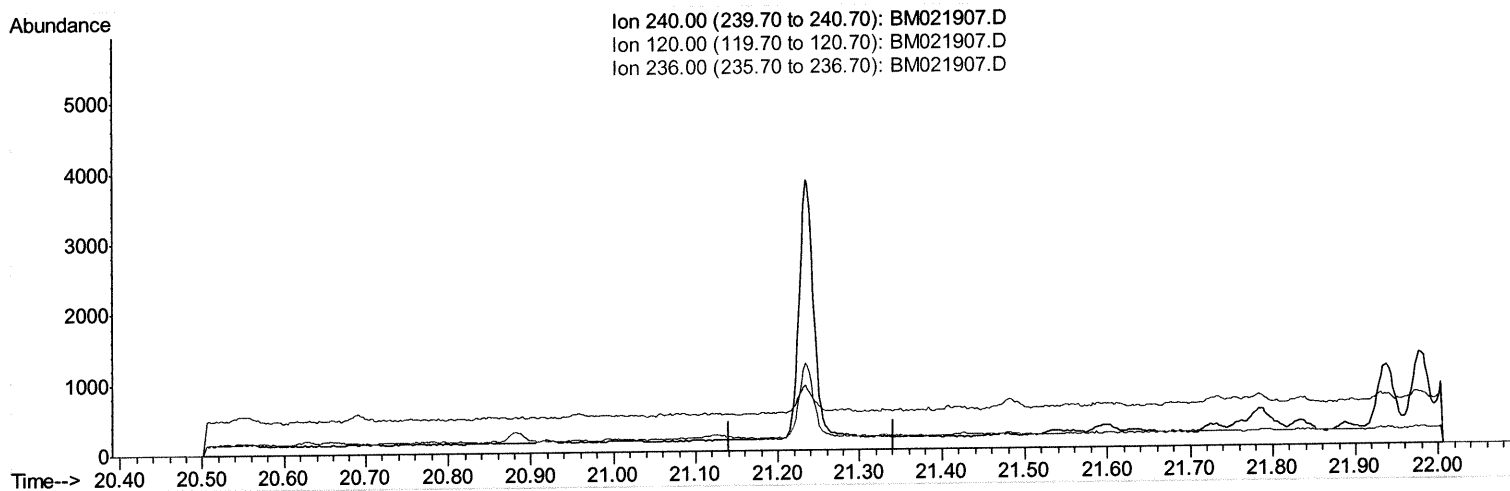

(16) Chrysene-d12 (I)

21.241min (-21.241) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:34:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

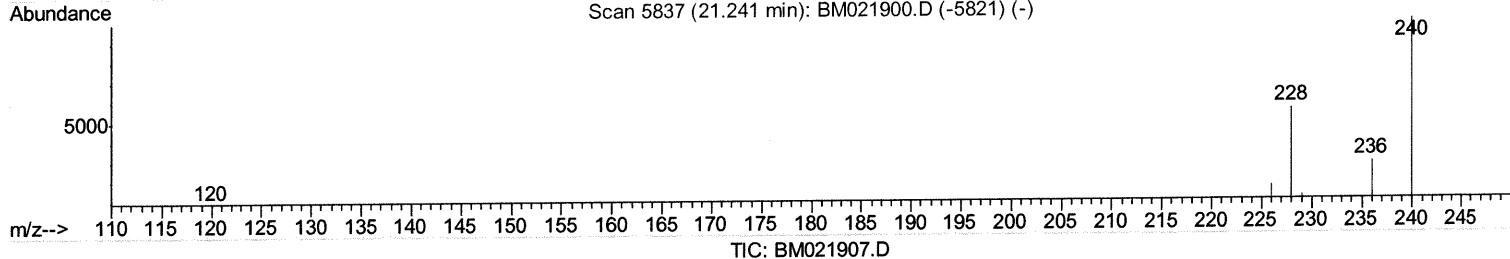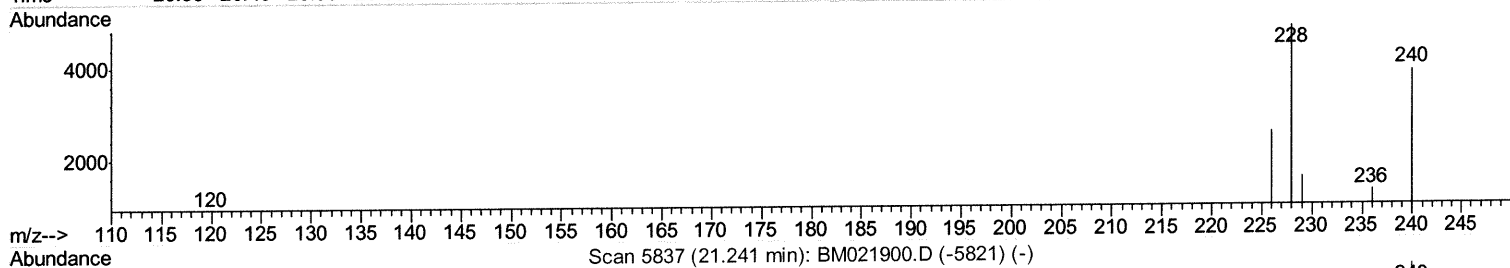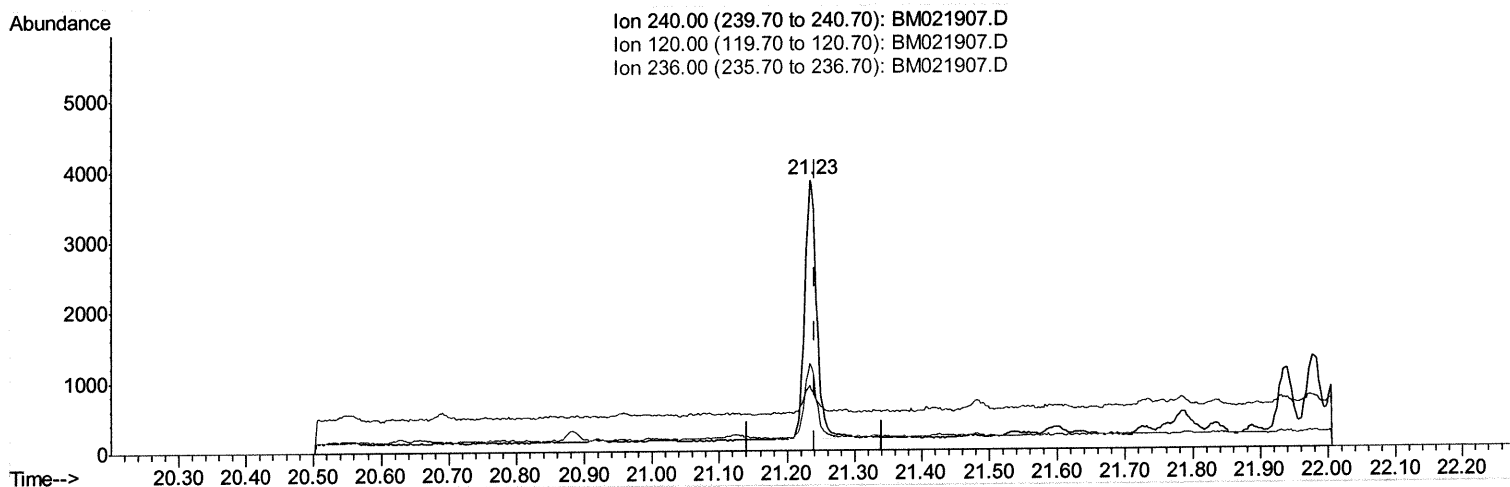

(16) Chrysene-d12 (I)

21.234min (-0.008) 0.40ng/ul m

JU
08/08/19

response 4537

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	24.04#
236.00	32.30	32.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:36:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

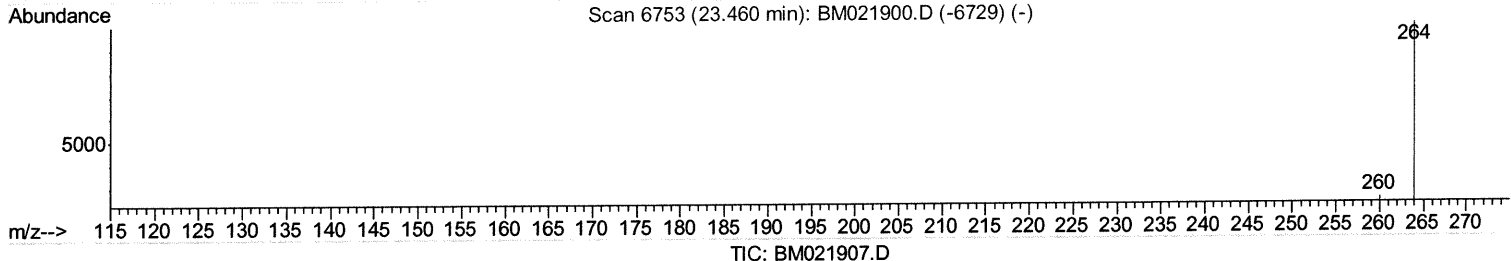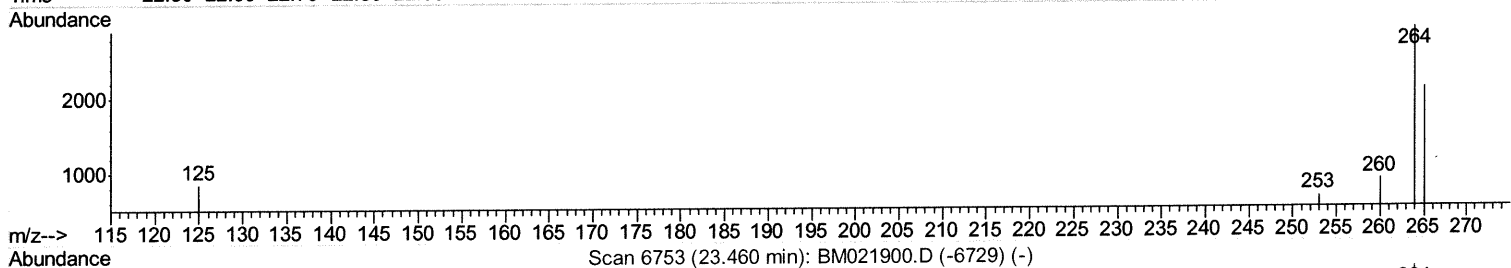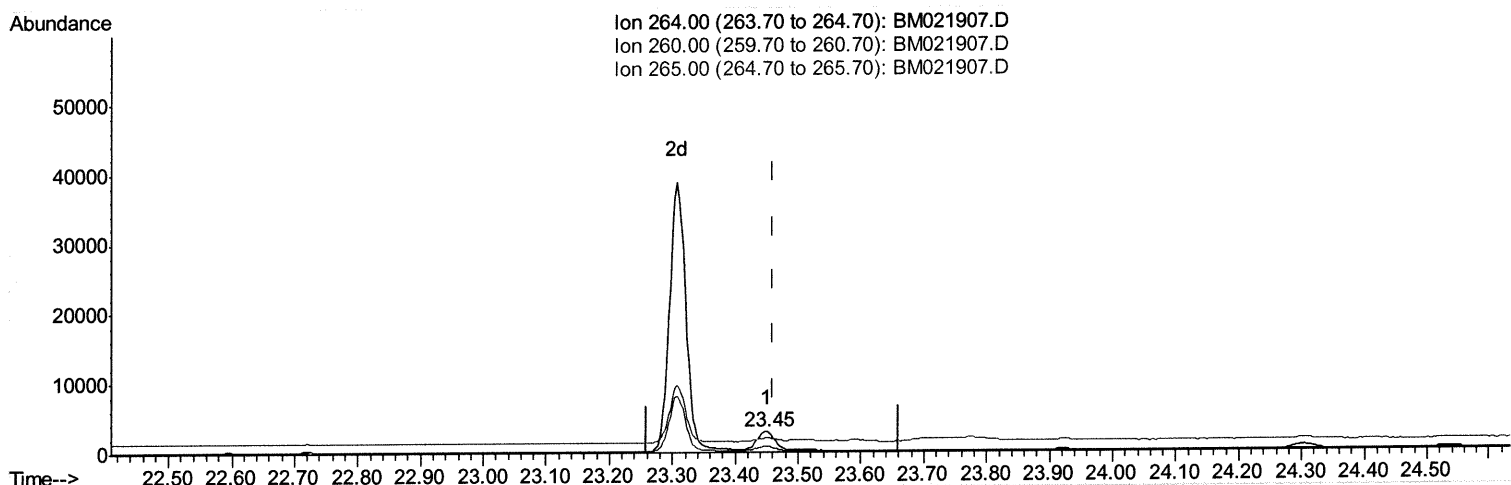

(20) Perylene-d12 (I)

23.450min (-0.010) 0.40ng/ul

response 6256

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	29.83
265.00	117.00	71.99#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:36:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

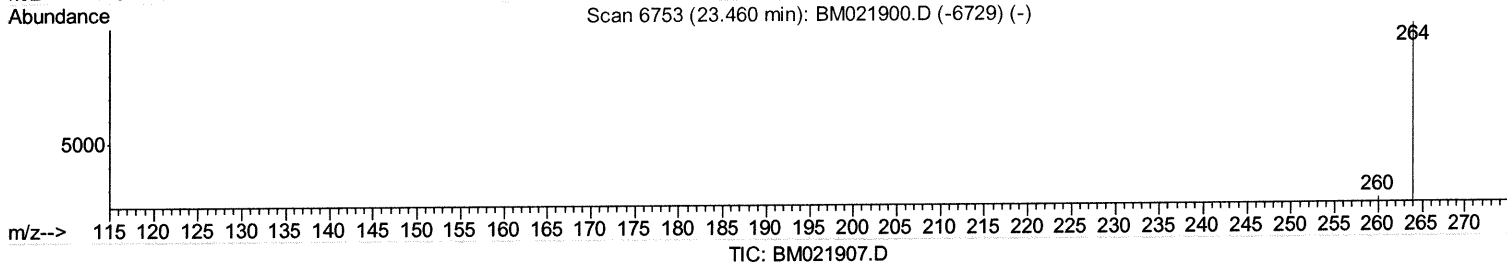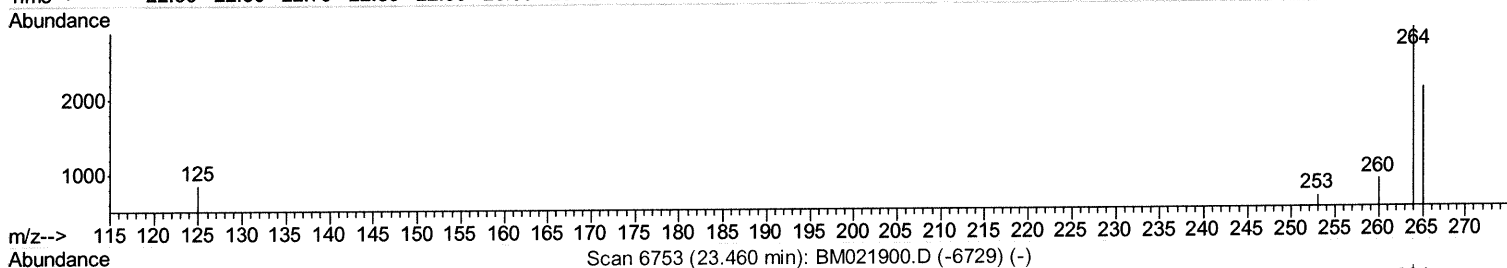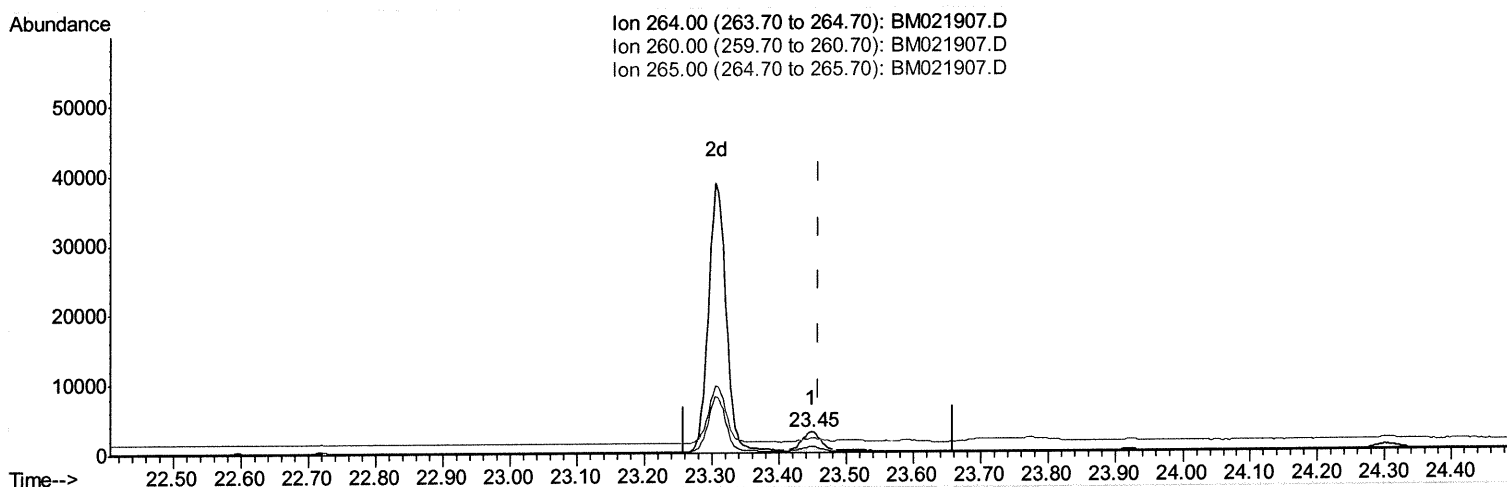

(20) Perylene-d12 (I)

23.450min (-0.010) 0.40ng/ul m

JU 08/08/19

response 4926

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	29.83
265.00	117.00	71.99#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:37:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

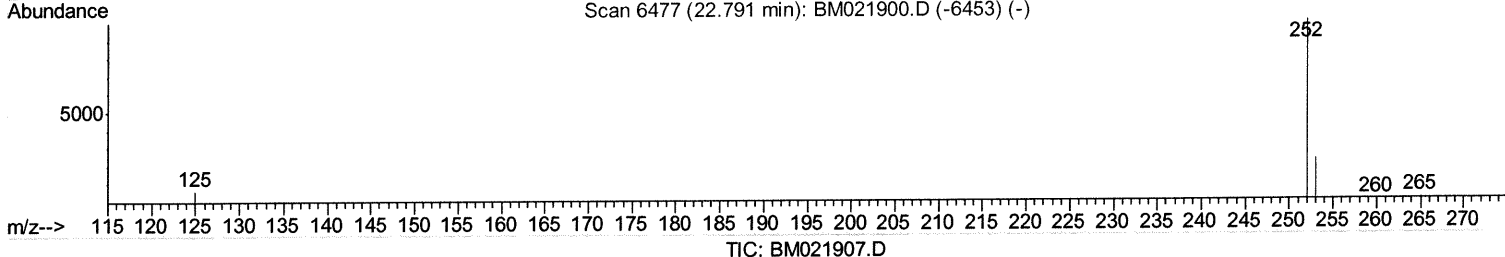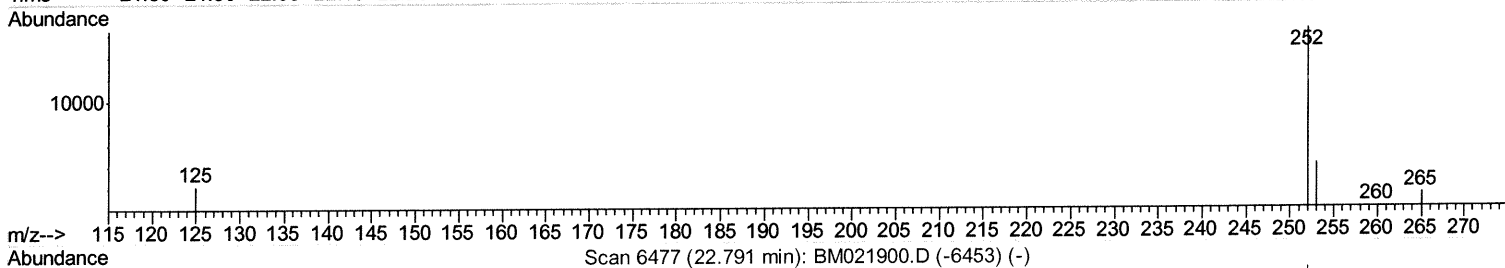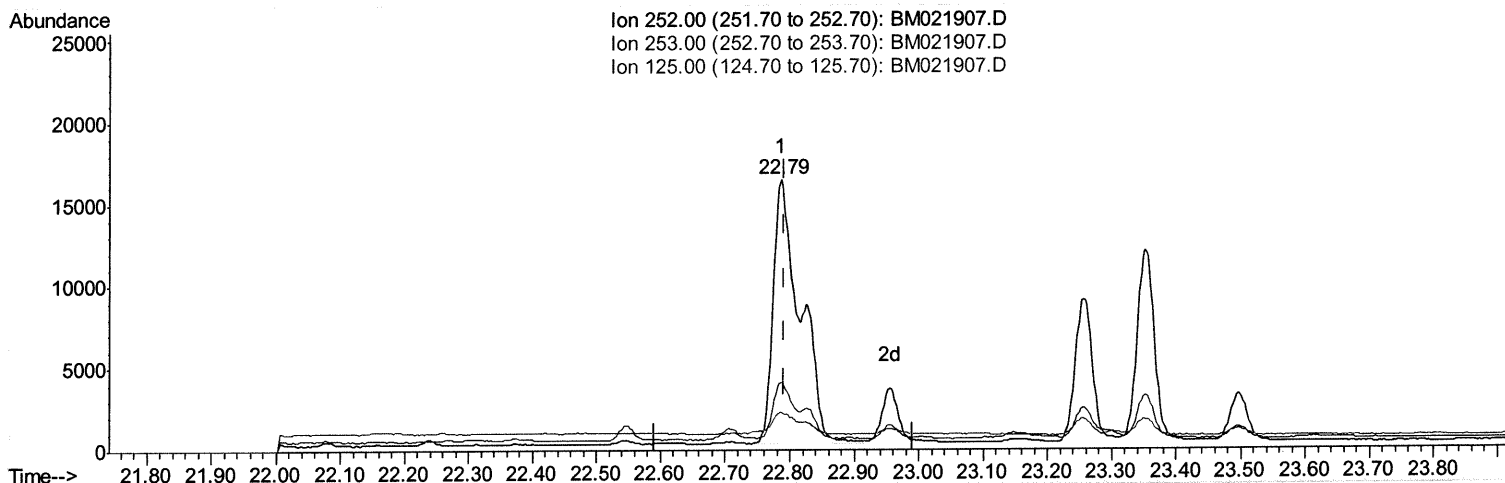

(21) Benzo(b)fluoranthene

22.786min (-0.005) 2.82ng/ul

response 46764

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.12
125.00	15.50	13.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)



Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:37:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

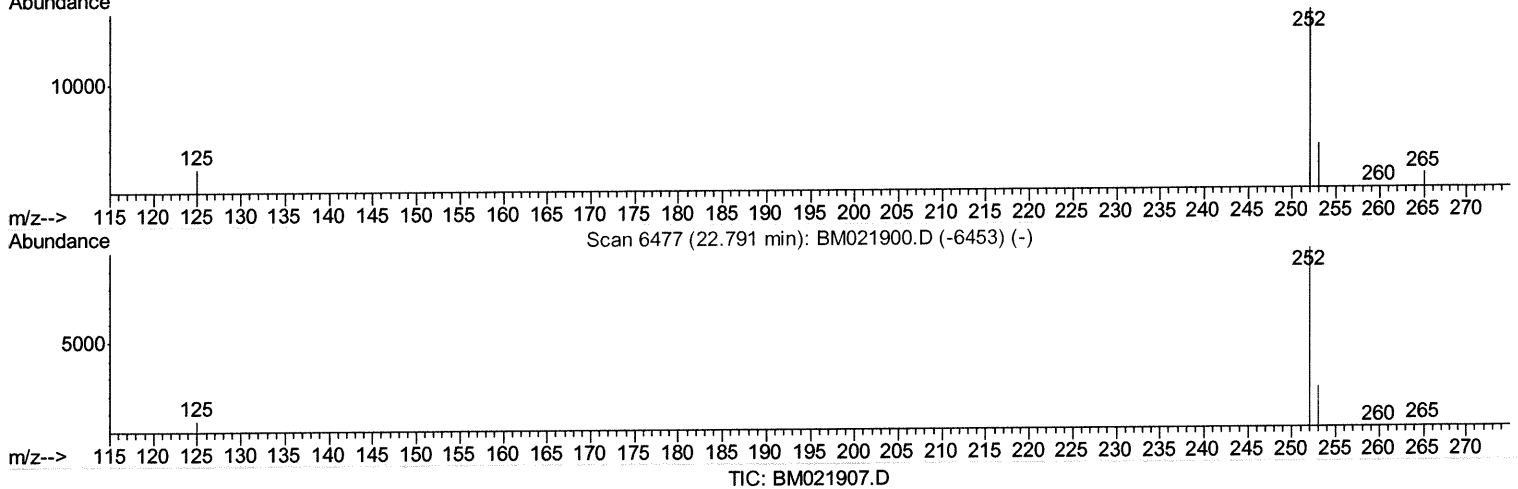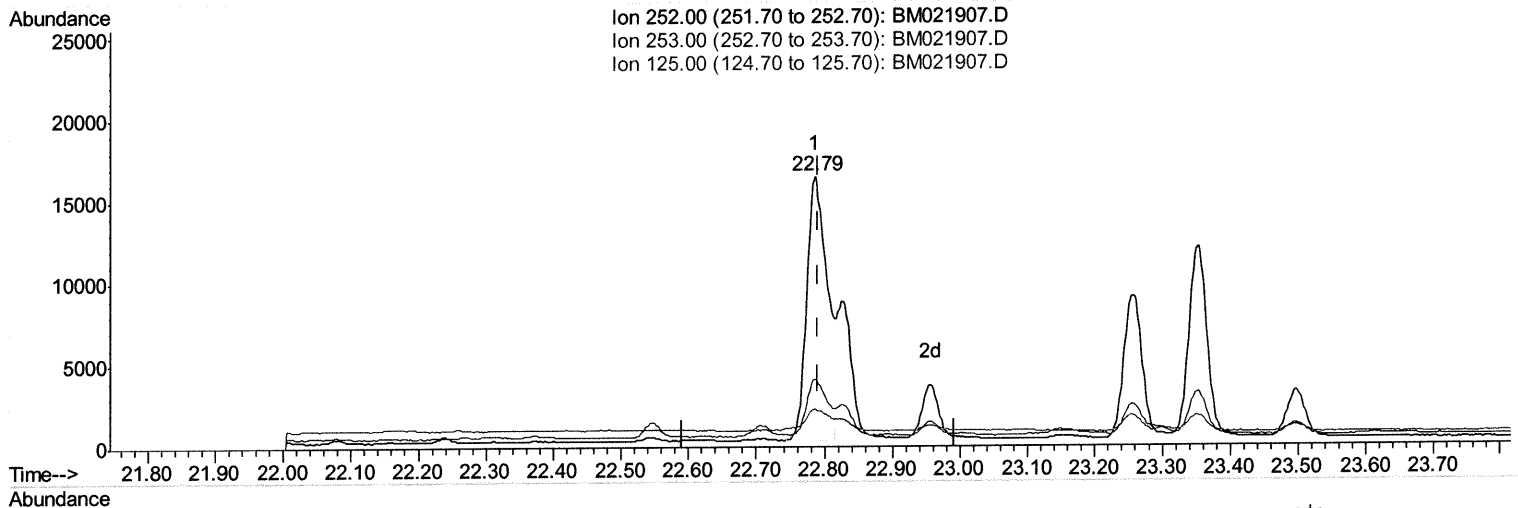

(21) Benzo(b)fluoranthene

22.786min (-0.005) 2.03ng/ul m

JU
08/08/19

response 33684

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.12
125.00	15.50	13.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:37:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

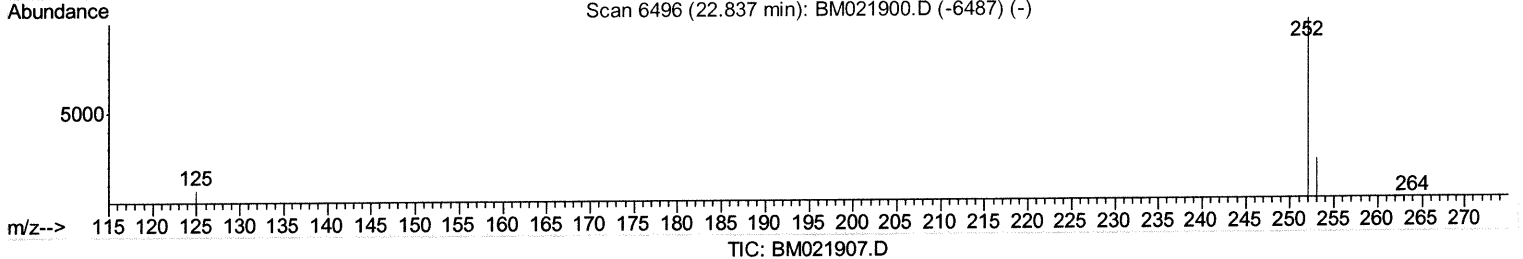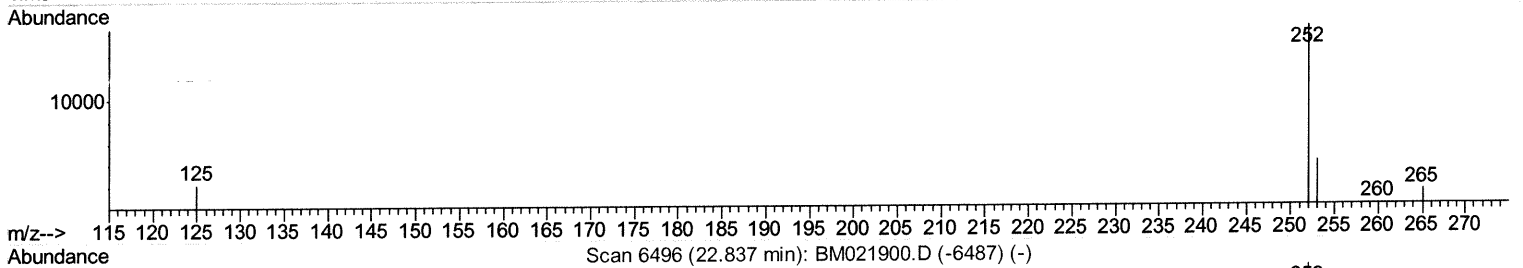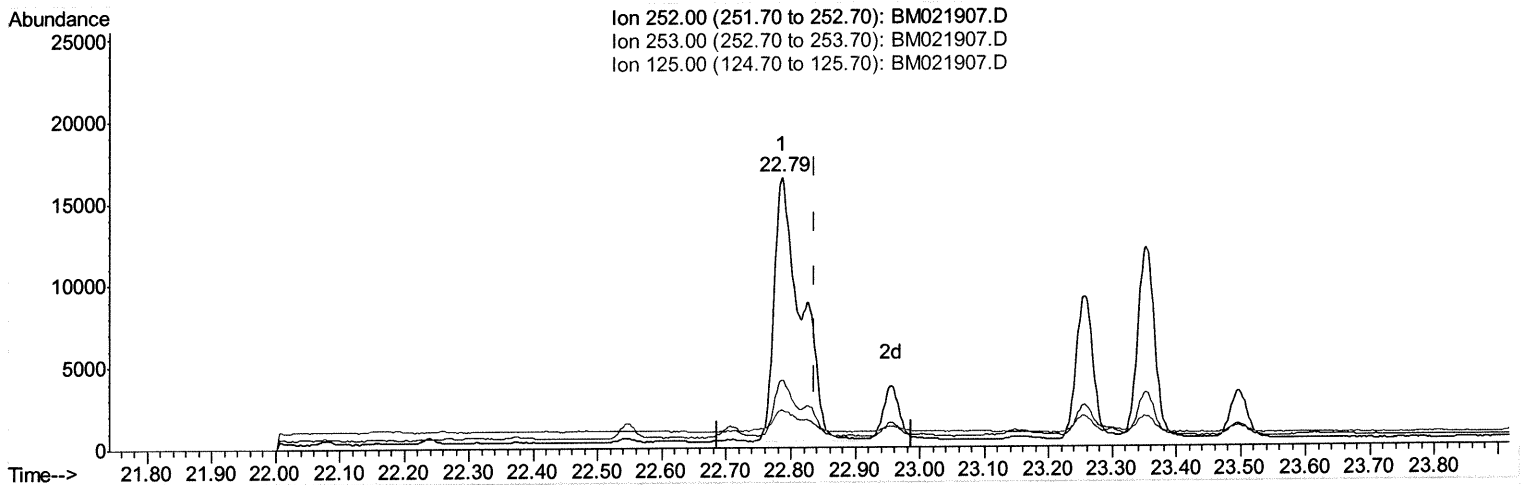

(22) Benzo(k)fluoranthene
22.786min (-0.051) 2.49ng/ul
response 46764
Ion Exp% Act%
252.00 100 100
253.00 33.70 25.12#
125.00 15.20 13.93
0.00 0.00 0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (Qedit)




Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:37:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

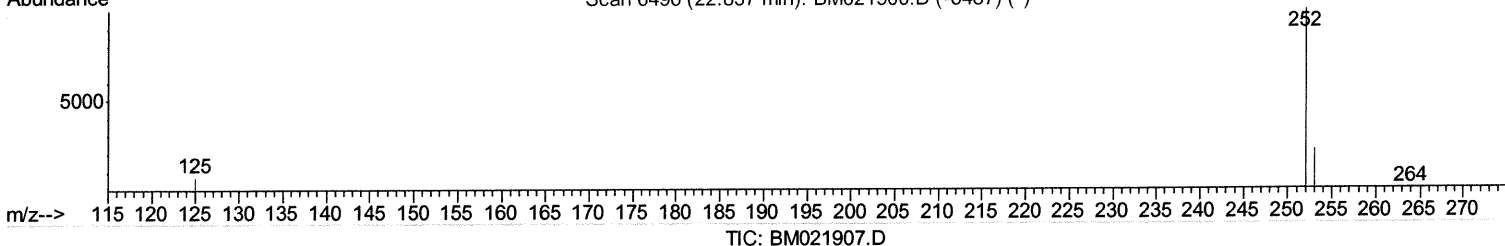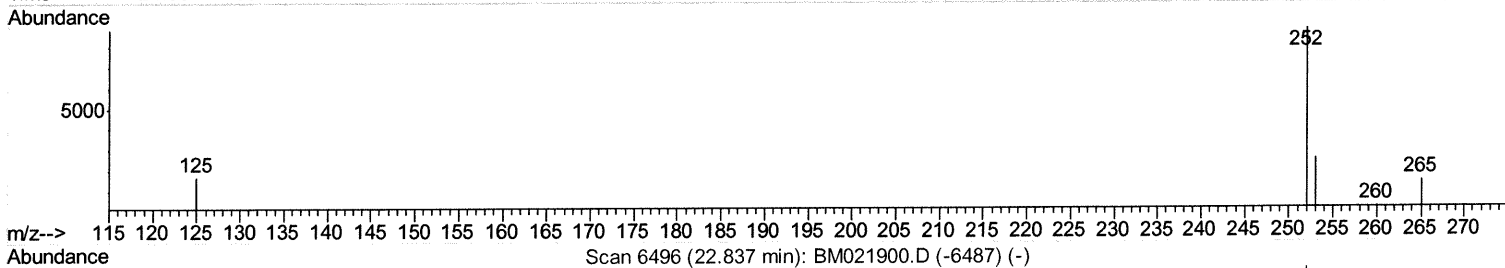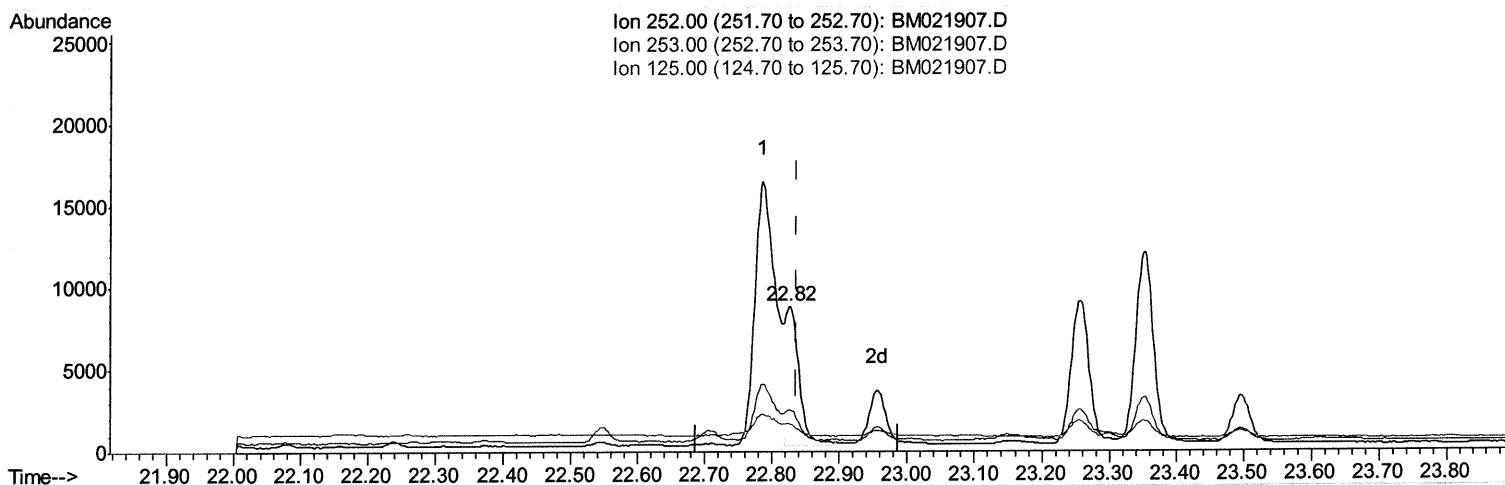

(22) Benzo(k)fluoranthene

22.825min (-0.012) 0.64ng/ul m

JU
08/08/19

response 12083

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	28.67
125.00	15.20	19.14#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
Quantitation Report (QT Reviewed)

Data File : BM021907.D
Acq On : 07 Aug 2019 21:56
Operator : HP/JU
Sample : K3893-12DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
BEP16DL

Manual Integrations
APPROVED

mohammad
8/9/2019 6:10:52 AM

Quant Time: Aug 08 05:37:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:13 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	790	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	3358	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	1978	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	4820m →	0.40	ng/ul	0.01
16) Chrysene-d12	21.23	240	4537m →	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	4926m →	0.40	ng/ul	0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	276	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	852m →	0.05	ng/ul	-0.01

Target Compounds

					Qvalue
3) Naphthalene	10.46	128	778	0.082	ng/ul# 83
5) 2-Methylnaphthalene	12.09	142	511	0.081	ng/ul 98
7) Acenaphthylene	14.00	152	2900	0.314	ng/ul# 84
8) Acenaphthene	14.34	153	520	0.069	ng/ul 95
9) Fluorene	15.34	166	785	0.094	ng/ul# 97
12) Phenanthrene	17.08	178	14816m →	1.056	ng/ul → 2JU
13) Anthracene	17.17	178	4283m →	0.358	ng/ul → JU 08/08/19
15) Fluoranthene	19.10	202	43703m →	2.326	ng/ul → JU
17) Pyrene	19.46	202	35613	1.910	ng/ul 99
18) Benzo(a)anthracene	21.22	228	22398	1.380	ng/ul 97
19) Chrysene	21.27	228	23360	1.119	ng/ul 97
21) Benzo(b)fluoranthene	22.79	252	33684m →	2.028	ng/ul → 2JU
22) Benzo(k)fluoranthene	22.82	252	12083m →	0.643	ng/ul → JU 08/08/19
23) Benzo(a)pyrene	23.35	252	21618	1.280	ng/ul# 84
24) Indeno(1,2,3-cd)pyrene	25.66	276	17781	0.882	ng/ul# 94
25) Dibenzo(a,h)anthracene	25.67	278	4526	0.278	ng/ul# 85
26) Benzo(g,h,i)perylene	26.34	276	15015	0.827	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed