
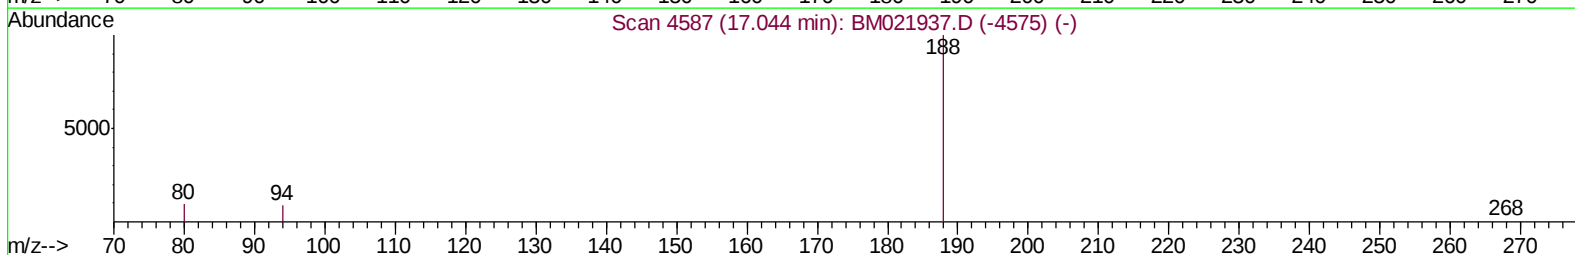
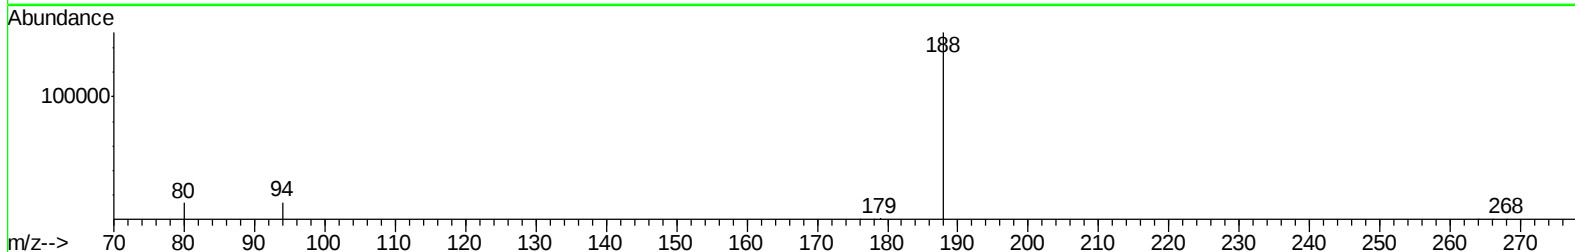


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:52:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

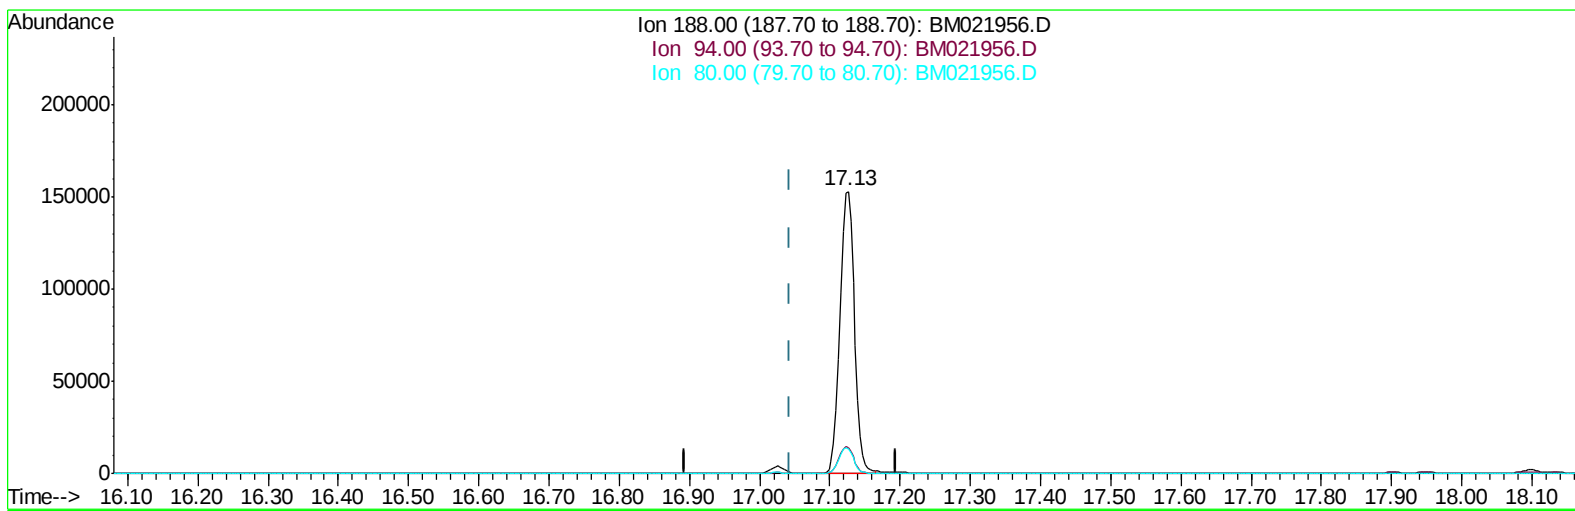

TIC: BM021956.D

(10) Phenanthrene-d10 (I)




17.126min (+0.082) 0.40ng/ul

response 217739

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.23
80.00	11.40	8.86#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:52:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

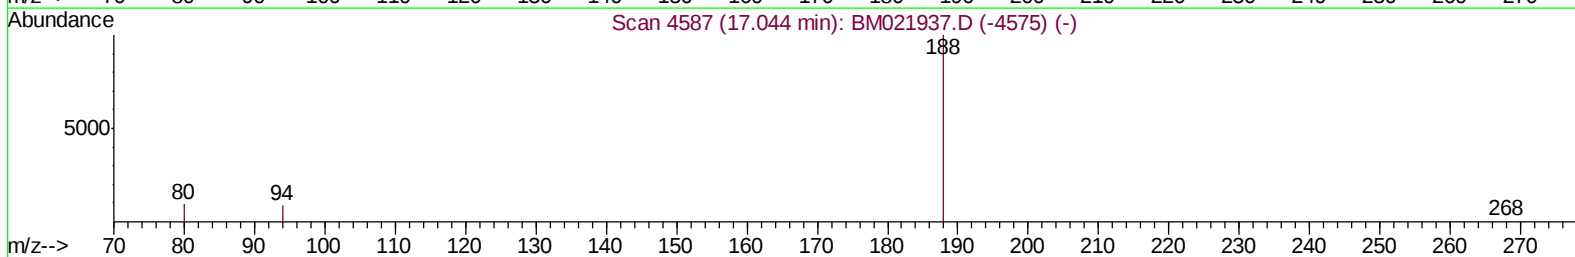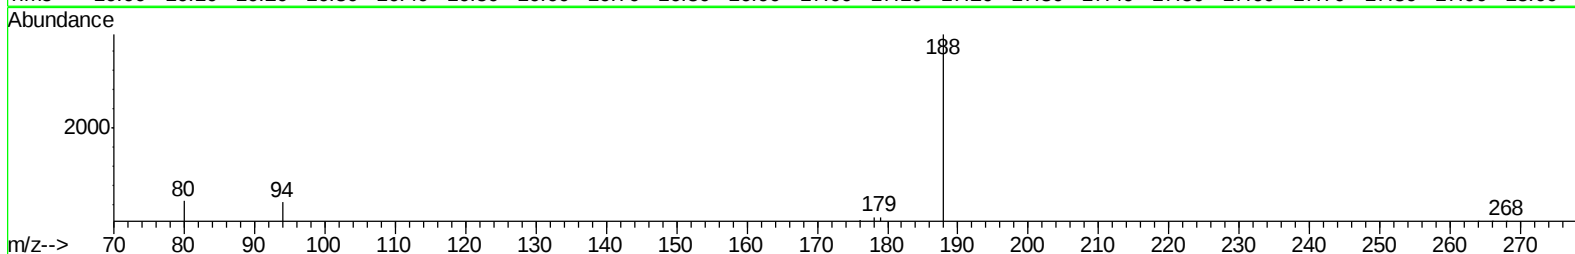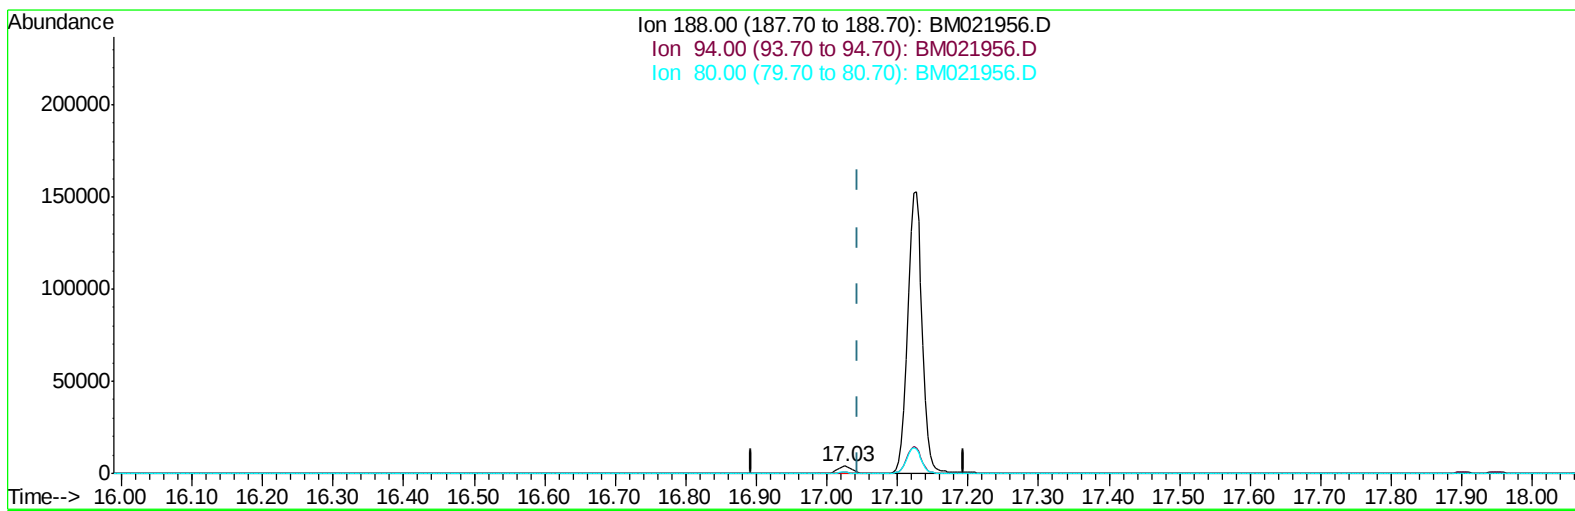

TIC: BM021956.D

(10) Phenanthrene-d10 (I)




17.025min (-0.019) 0.40ng/ul m

response 5599

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.23
80.00	11.40	11.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

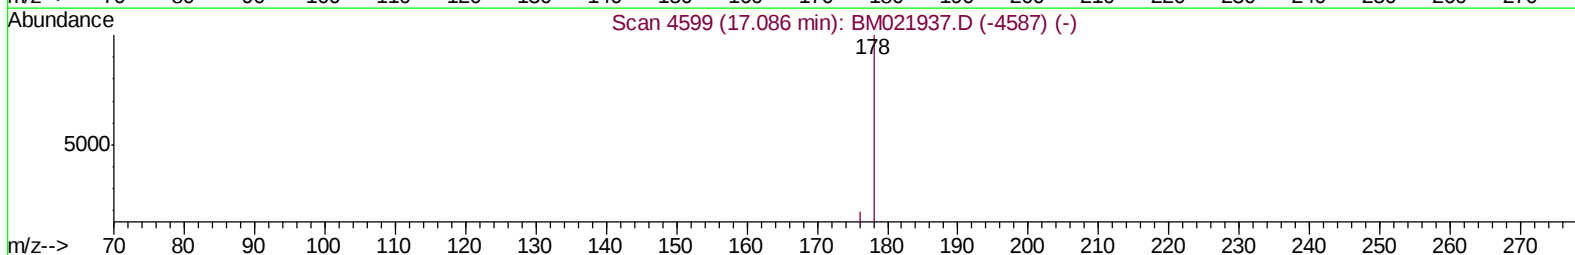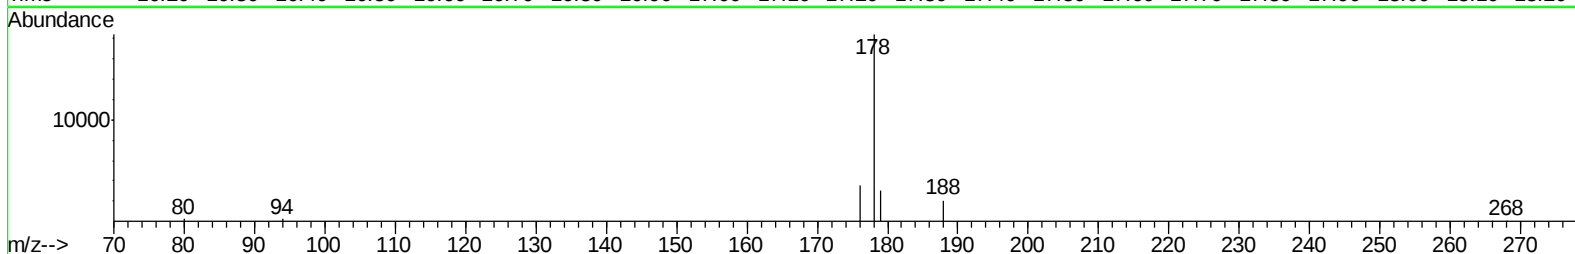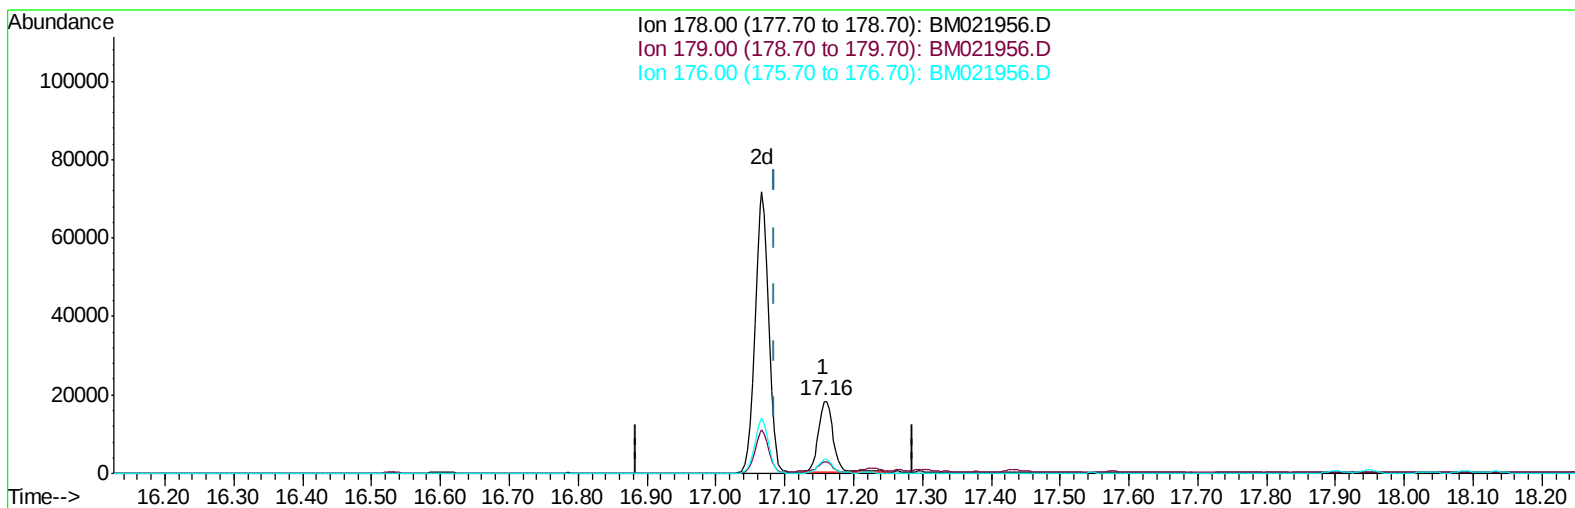

TIC: BM021956.D

(12) Phenanthrene




17.157min (+0.071) 1.67ng/ul

response 27150

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	16.42
176.00	21.00	19.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

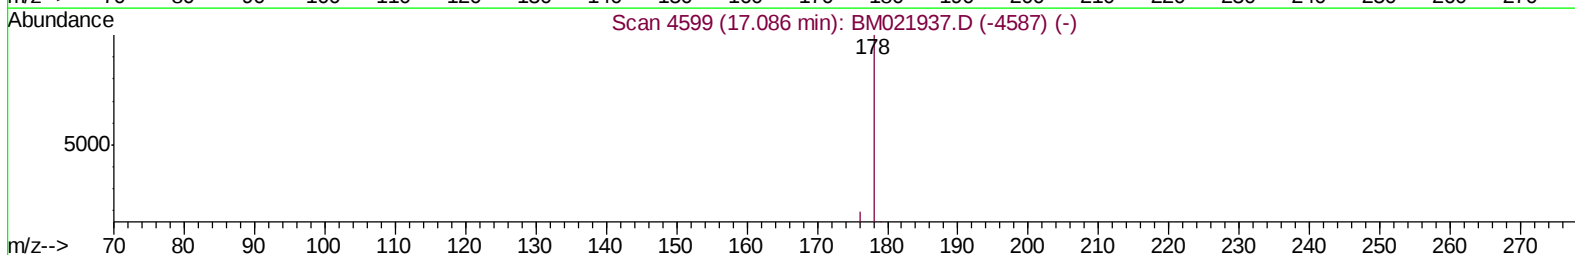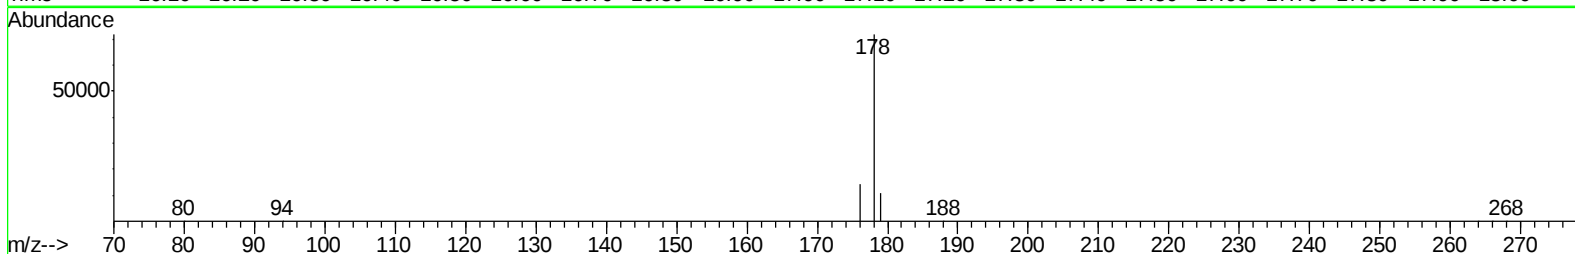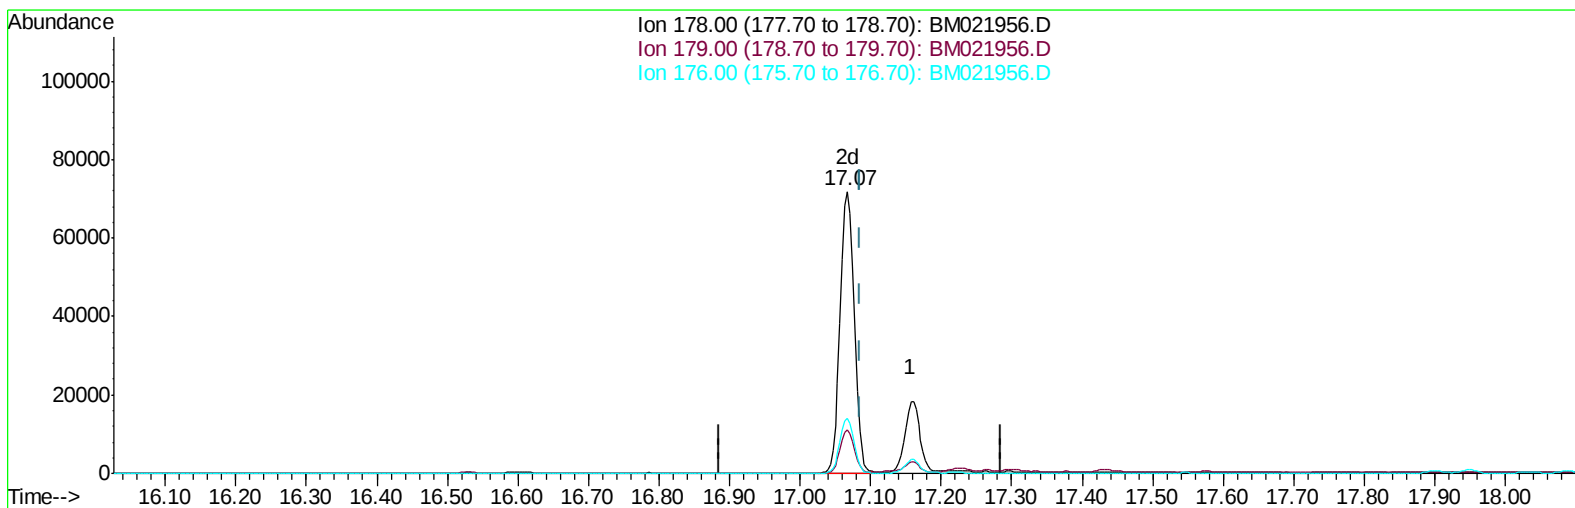

TIC: BM021956.D

(12) Phenanthrene




17.067min (-0.019) 6.06ng/ul m

response 98783

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	15.41
176.00	21.00	19.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

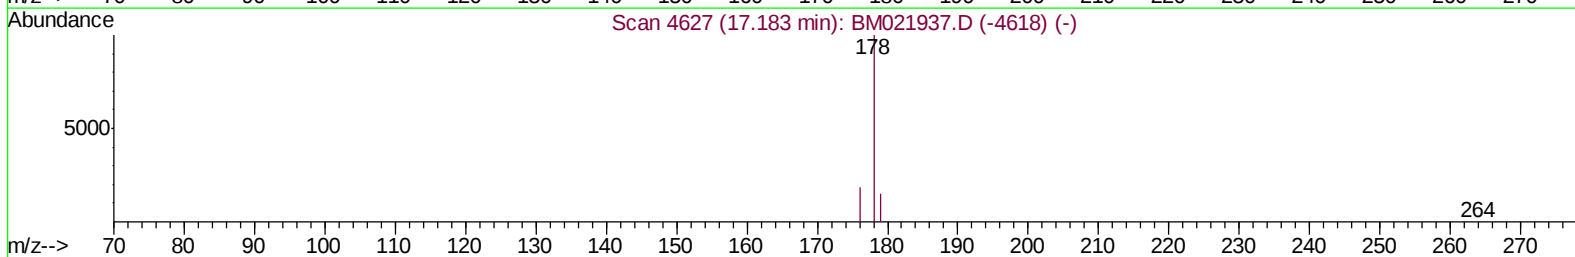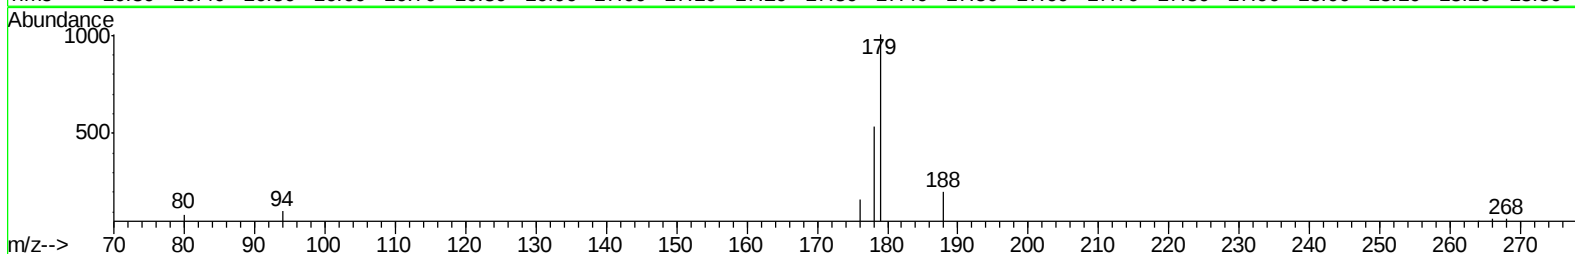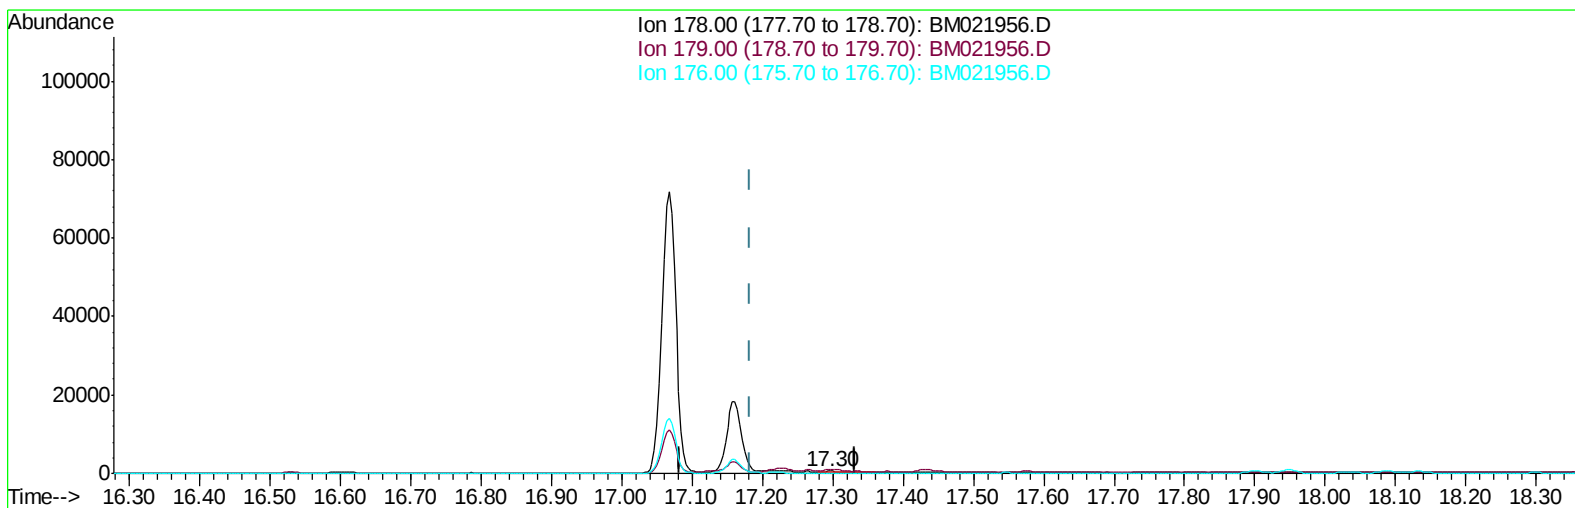

TIC: BM021956.D

(13) Anthracene




17.296min (+0.113) 0.05ng/ul

response 761

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	187.31#
176.00	20.80	30.78#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

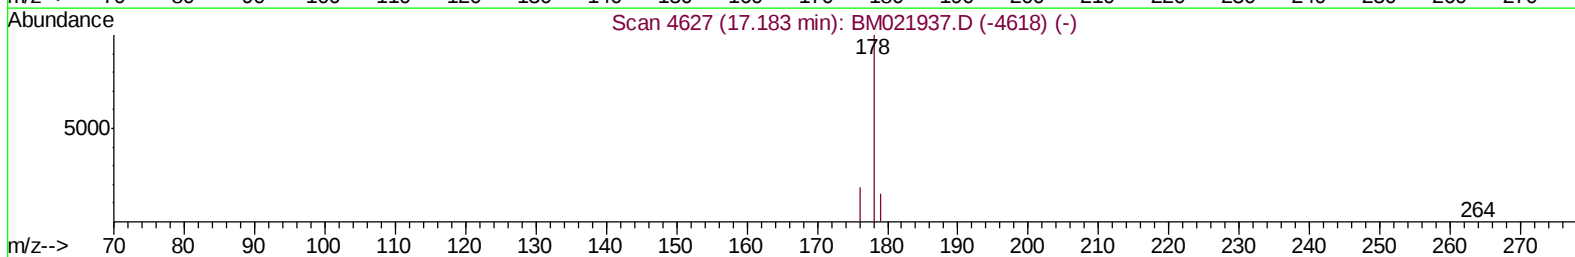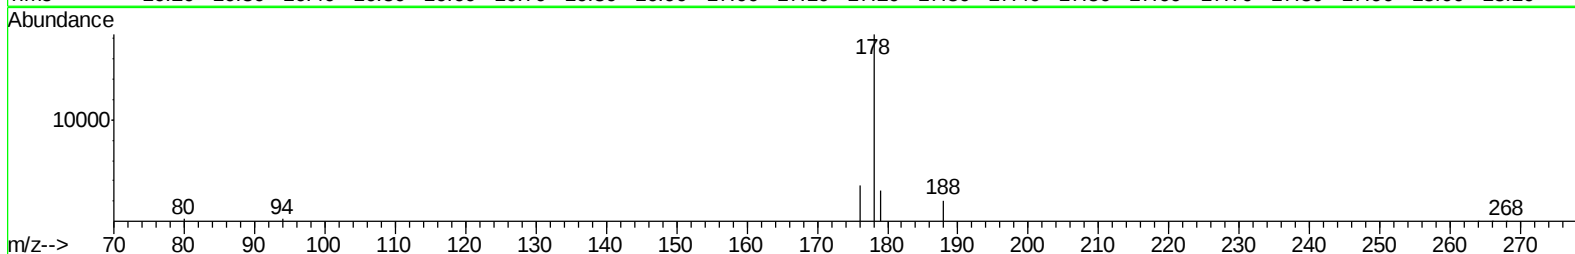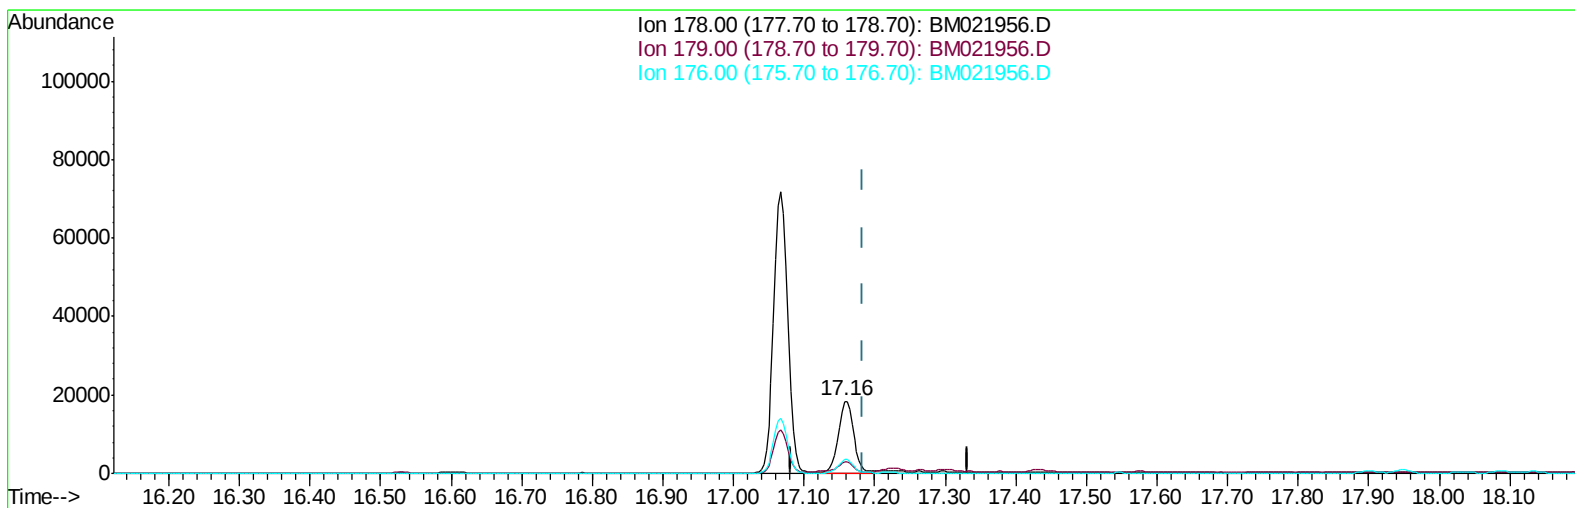

TIC: BM021956.D

(13) Anthracene




17.157min (-0.026) 1.99ng/ul m

response 27595

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	16.42
176.00	20.80	19.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

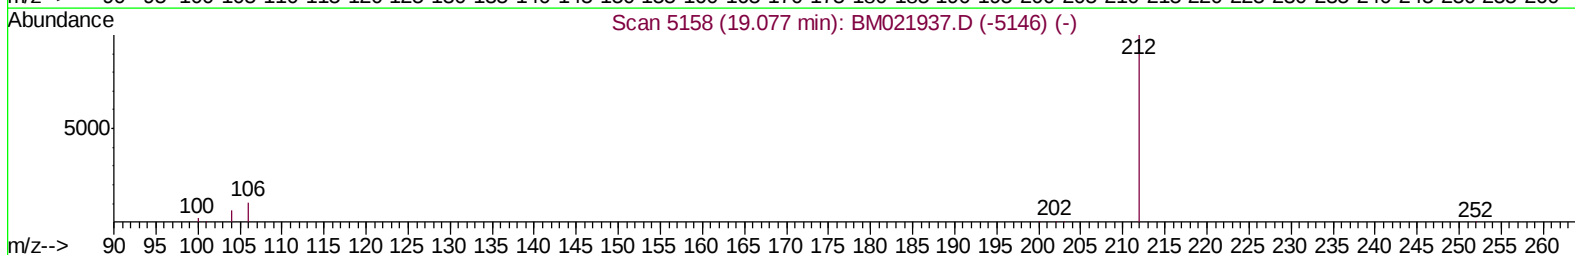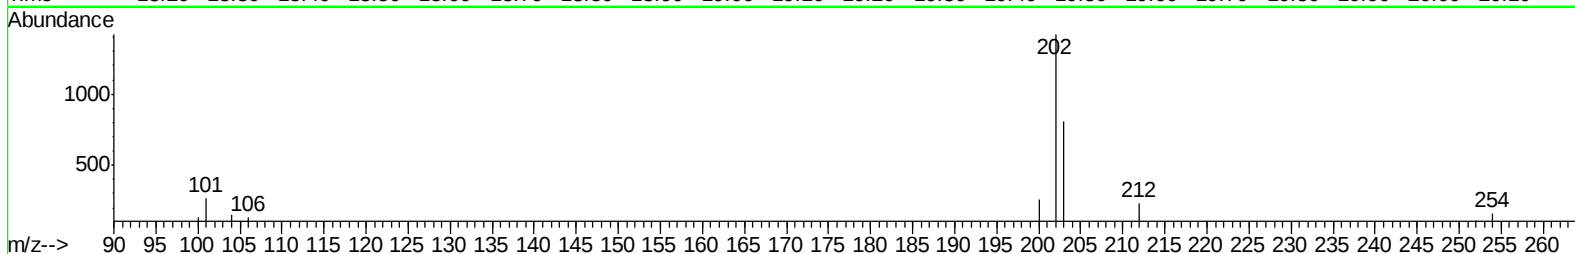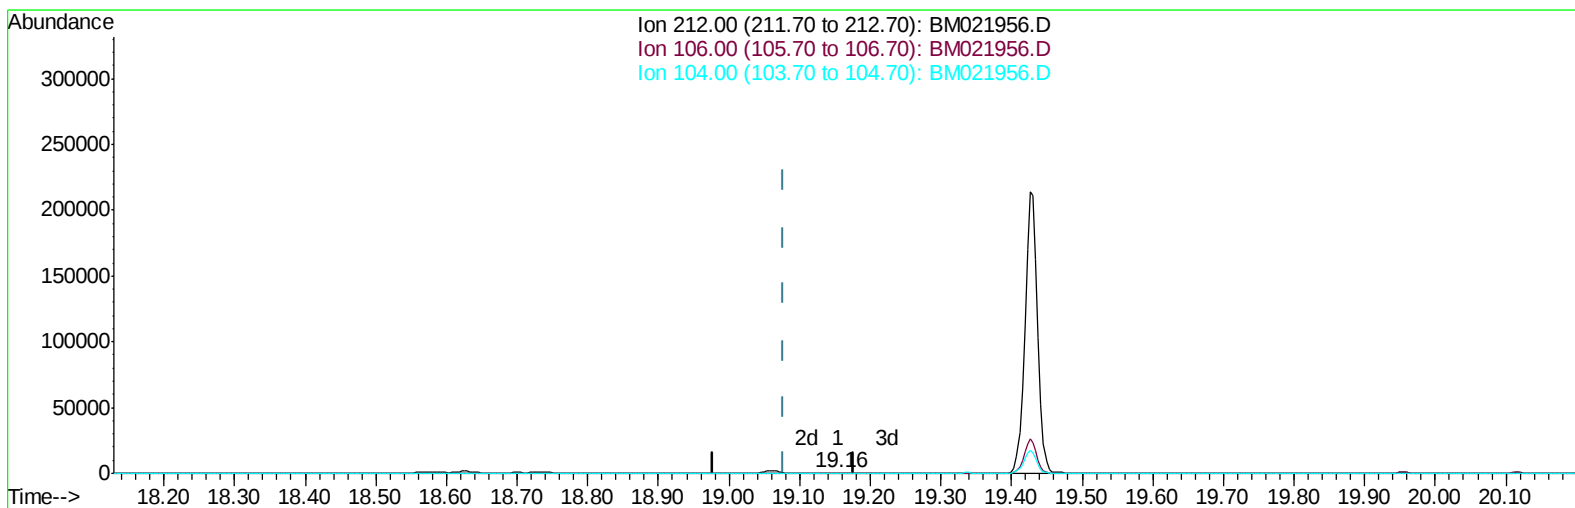

TIC: BM021956.D

(14) Fluoranthene-d10 (SURRE)




19.156min (+0.079) 0.01ng/ul

response 237

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	6.75#
104.00	6.00	56.96#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

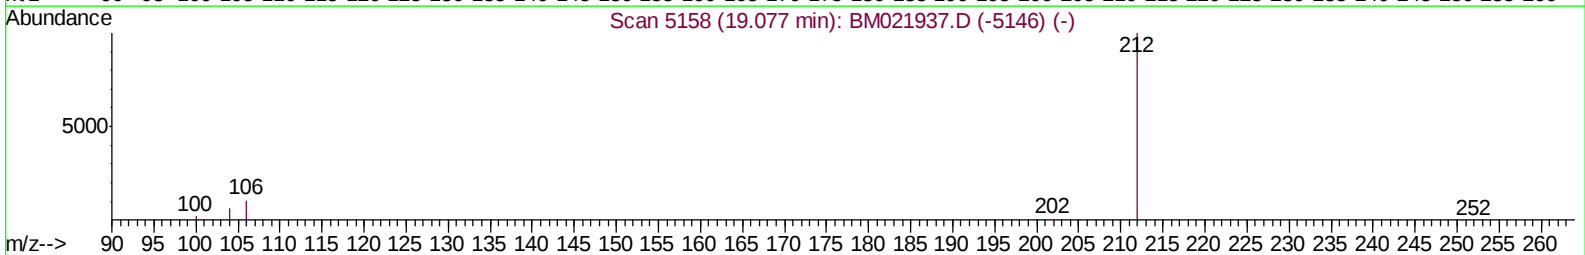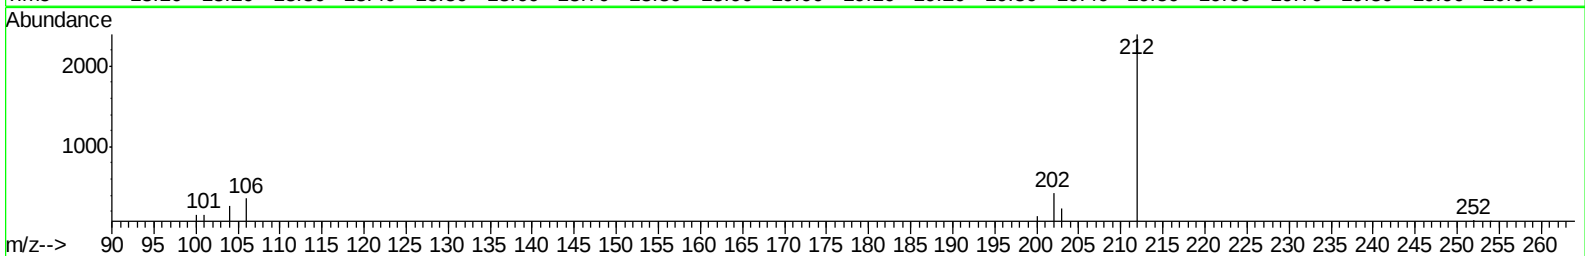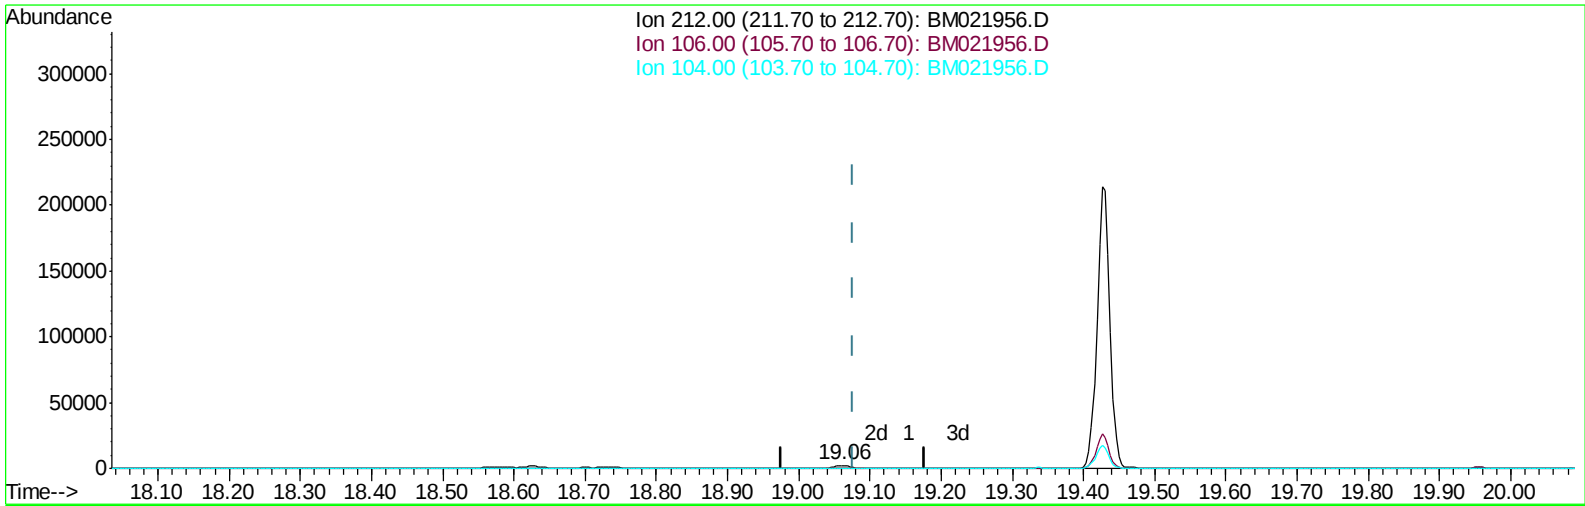

TIC: BM021956.D

(14) Fluoranthene-d10 (SURRE)




19.060min (-0.017) 0.18ng/ul m

response 3428

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.47#
104.00	6.00	3.94#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080719\
Data File : BM021956.D
Acq On : 09 Aug 2019 06:16
Operator : HP/JU
Sample : K4028-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 09 13:53:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

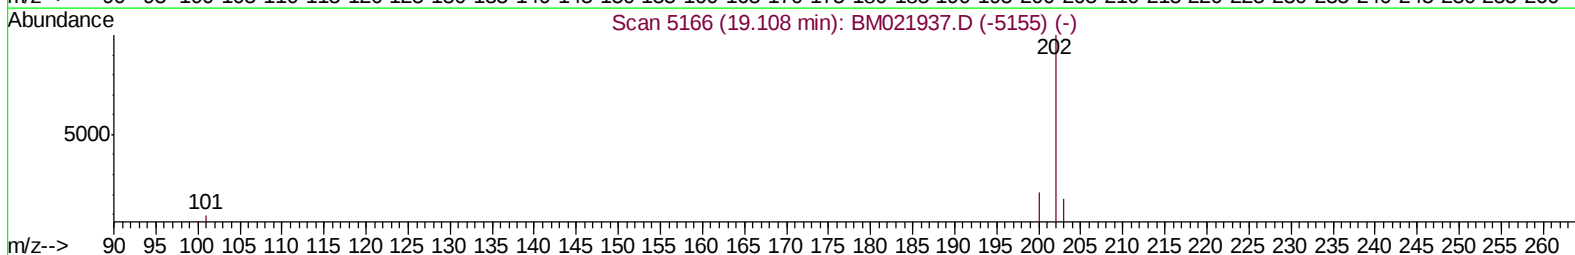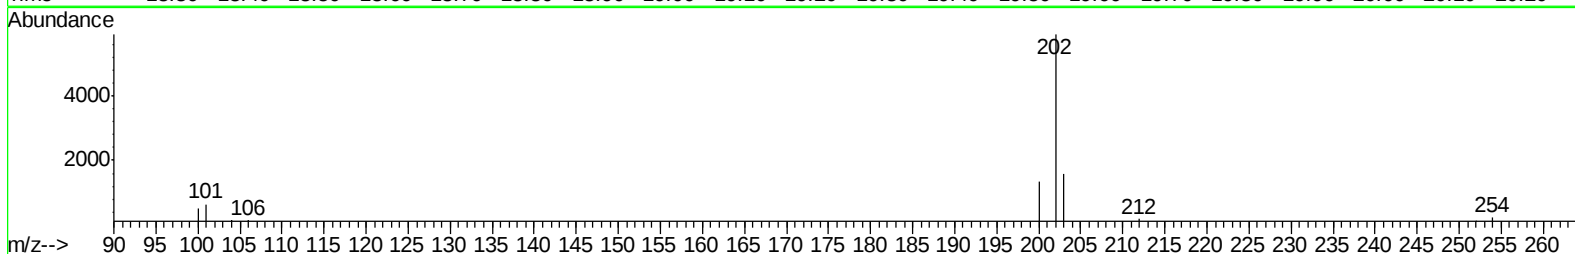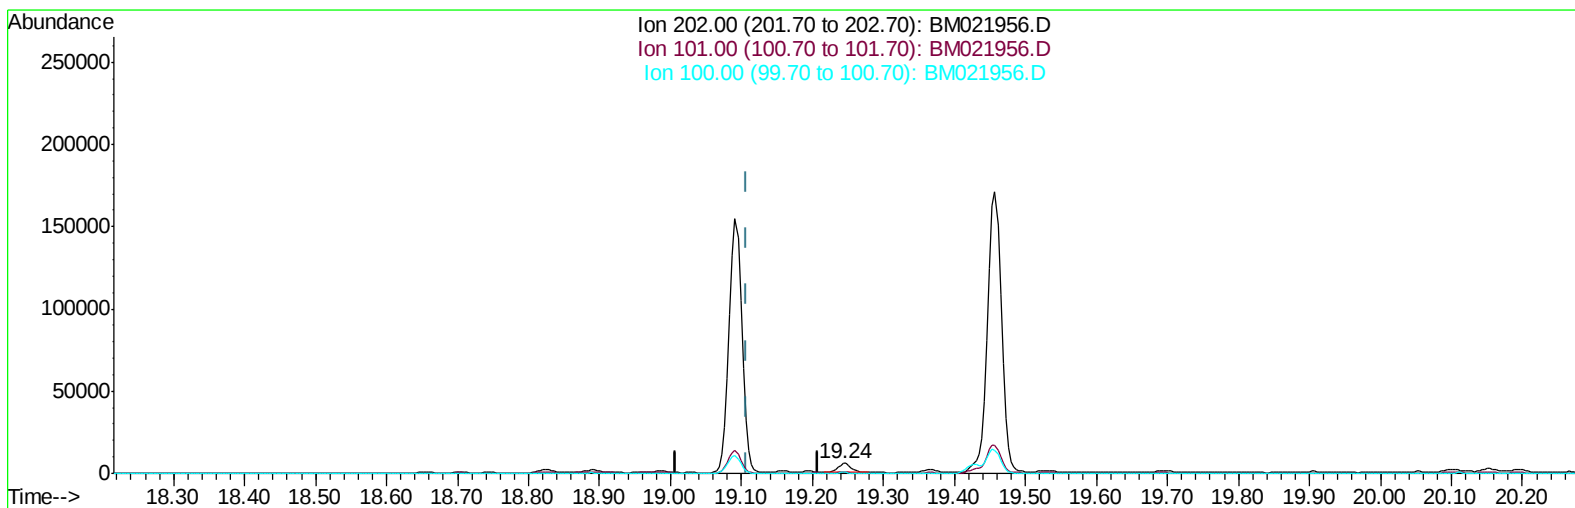

TIC: BM021956.D

(15) Fluoranthene (C)

19.244min (+0.136) 0.34ng/ul

response 7343

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	10.68
100.00	8.10	8.40
0.00	0.00	0.00