


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080719\
 Data File : BM021890.D
 Acq On : 07 Aug 2019 11:34
 Operator : HP/JU
 Sample : DFTPP01
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP01

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 18:27:47 2019

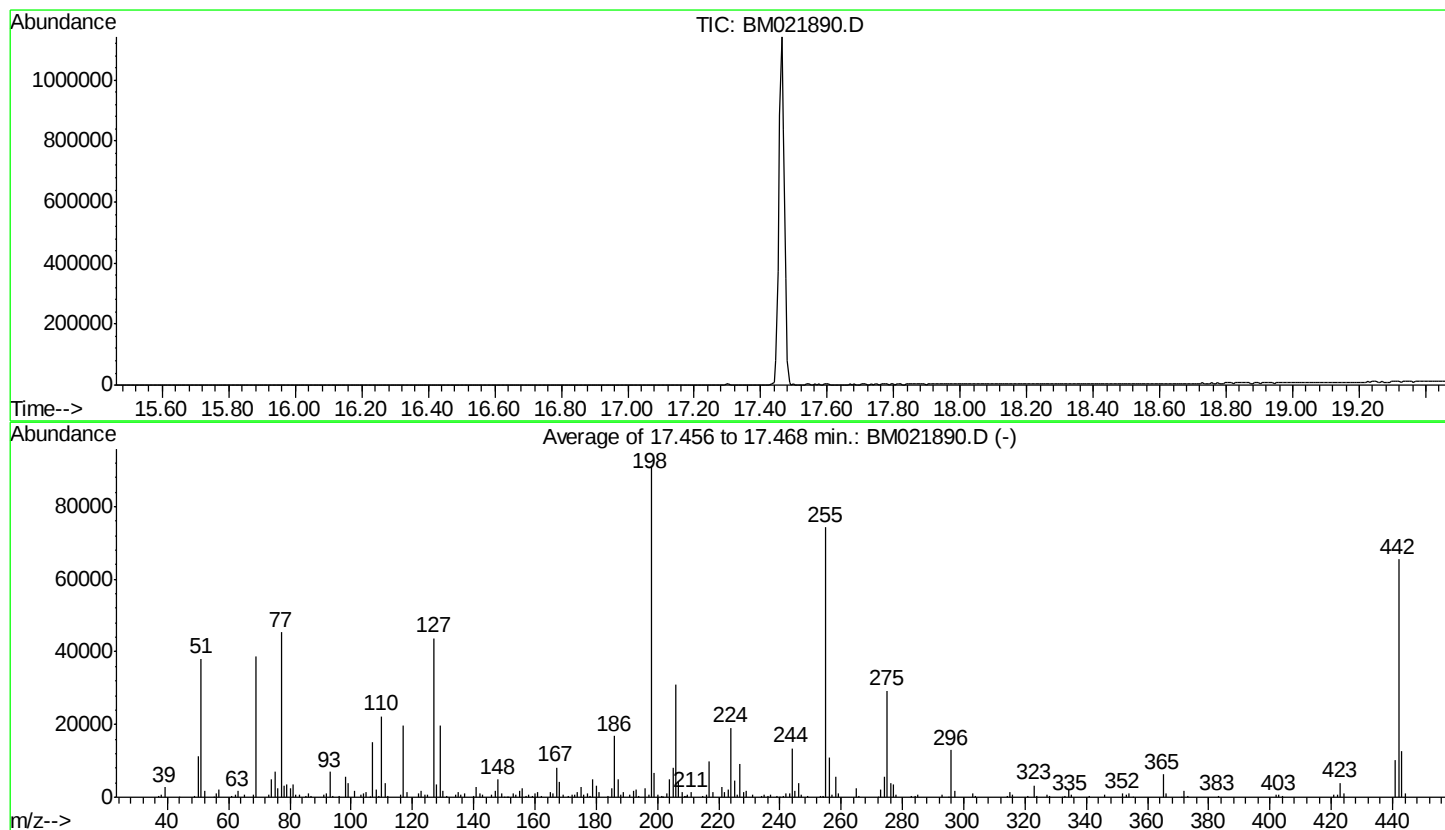

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	38136	PASS
68	69	0.00	2	1.6	639	PASS
69	198	0.00	100	42.6	38834	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	43781	PASS
197	198	0.00	2	0.6	581	PASS
198	198	100	100	100.0	91240	PASS
199	198	5	9	7.2	6535	PASS
275	198	10	60	32.1	29309	PASS
365	198	1	100	6.9	6336	PASS
441	198	0.01	100	11.2	10228	PASS
442	198	50	100	71.6	65368	PASS
443	442	15	24	19.3	12616	PASS

m/z	Abundance
36.90	319.0
38.00	483.0
39.00	3041.0
40.00	322.0
43.90	714.0
48.90	392.0
50.00	12041.0
51.00	40520.0
52.00	1987.0
56.00	988.0
57.00	2299.0
61.00	598.0
62.00	608.0
63.00	1839.0
65.00	657.0
68.10	693.0
69.00	40328.0
73.00	808.0
74.00	5039.0
75.00	7559.0
76.00	2657.0
77.00	47584.0
78.00	3711.0
79.00	3646.0
80.00	2687.0
81.00	3270.0
82.00	746.0
83.00	736.0
85.00	486.0
86.00	1173.0
87.00	603.0
90.90	782.0
92.00	1185.0
93.00	6983.0
94.00	538.0
95.90	450.0
98.00	5709.0
99.00	4270.0
101.00	1509.0
102.90	662.0
104.00	1237.0
105.00	1507.0
107.00	15640.0
108.00	2407.0
109.00	707.0
110.00	22648.0
111.00	3896.0
112.00	552.0
115.90	862.0
117.00	19432.0
118.00	1470.0
122.00	910.0
122.90	1518.0
124.00	781.0
124.90	624.0
127.00	42304.0
128.00	3627.0
129.00	19448.0
130.00	1749.0
131.00	328.0
134.00	719.0
135.00	1622.0
136.00	665.0
137.00	910.0
140.00	342.0
141.00	3239.0
142.00	1054.0
142.90	689.0
145.90	621.0
147.00	1788.0
148.00	4764.0
149.00	1036.0
151.20	426.0
153.00	946.0
153.90	802.0
155.00	1486.0
156.00	2451.0
156.90	504.0
157.90	549.0
158.90	472.0
159.90	1127.0
160.90	1417.0
162.00	347.0
164.90	1373.0
165.90	779.0
167.00	7664.0
168.00	4382.0
169.00	622.0
170.90	337.0
171.90	639.0
172.90	735.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

173.90	1321.0
175.00	2710.0
175.90	654.0
177.00	1256.0
178.00	569.0
178.90	5258.0
180.00	3337.0
181.00	1556.0
183.90	481.0
184.90	2302.0
186.00	15649.0
187.00	4518.0
188.00	585.0
188.90	1177.0
190.90	644.0
192.00	1734.0
193.00	1836.0
193.90	325.0
196.00	2226.0
197.10	583.0
197.90	84448.0
198.90	6265.0
199.90	580.0
201.20	412.0
201.70	335.0
203.00	906.0
204.00	4702.0
205.00	7286.0
206.00	28712.0
207.00	4760.0
208.00	1225.0
208.90	671.0
209.90	638.0
211.00	1156.0
214.90	441.0
216.00	876.0
216.90	8749.0
218.00	1229.0
220.90	2646.0
221.90	1139.0
223.00	1761.0
224.00	16568.0
225.00	4355.0
226.00	629.0
227.00	8217.0
227.90	1210.0
228.90	1835.0
230.90	640.0
233.80	438.0
234.90	689.0
236.00	450.0
236.90	905.0
238.90	410.0
241.00	453.0
242.00	837.0
243.00	1072.0
244.00	11535.0
245.00	1643.0
246.00	3424.0
247.00	734.0
248.90	422.0
253.00	374.0
253.90	400.0
255.00	63880.0
256.00	9428.0
256.90	864.0
258.00	5050.0
258.90	904.0
264.90	2059.0
265.90	403.0
273.00	2106.0
274.00	4978.0
275.00	24408.0
276.00	3444.0
277.00	3007.0
277.90	551.0
283.00	331.0
285.00	487.0
292.90	633.0
296.00	10969.0
297.00	1705.0
303.00	994.0
303.90	387.0
314.00	459.0
315.00	1179.0
315.90	658.0
323.00	2695.0
323.90	345.0
326.90	766.0
334.10	1853.0
334.90	611.0
341.00	511.0
345.90	569.0
352.00	641.0
352.90	435.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

354.00	742.0
365.00	4550.0
366.00	854.0
372.00	1064.0
382.90	365.0
402.00	395.0
402.90	522.0
420.90	445.0
422.10	557.0
423.00	2830.0
424.00	702.0
441.00	7025.0
442.00	45936.0
443.00	9593.0
444.00	667.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
37.00	310.0
38.00	762.0
39.00	3265.0
40.00	310.0
44.00	560.0
49.00	388.0
50.00	13067.0
51.00	44760.0
52.10	2034.0
55.00	348.0
56.00	1200.0
57.00	2638.0
61.00	442.0
62.00	756.0
63.00	1761.0
65.00	839.0
68.00	750.0
69.00	46760.0
73.00	1056.0
74.00	5940.0
75.00	8533.0
76.00	2739.0
77.10	53504.0
78.00	3793.0
79.00	4271.0
80.00	2506.0
81.00	4023.0
82.00	1014.0
82.90	854.0
85.00	584.0
86.00	1280.0
87.10	551.0
90.90	954.0
92.00	1174.0
93.00	8673.0
94.00	530.0
95.90	379.0
98.00	6996.0
99.00	4790.0
101.00	2225.0
103.00	736.0
104.00	1582.0
105.00	1493.0
105.90	409.0
107.00	17840.0
108.00	2559.0
109.00	529.0
110.00	26704.0
111.00	4310.0
112.00	667.0
116.00	1117.0
117.00	23280.0
118.00	1628.0
121.90	1385.0
123.00	2067.0
123.90	880.0
125.00	801.0
127.00	51792.0
128.00	3921.0
129.00	23744.0
130.00	2247.0
131.00	419.0
133.90	702.0
135.00	1809.0
136.00	826.0
137.00	1373.0
140.00	368.0
141.00	3258.0
142.00	1109.0
143.00	758.0
145.90	610.0
147.00	2075.0
148.00	5490.0
149.00	891.0
149.90	392.0
150.90	376.0
152.90	1135.0
153.90	844.0
155.00	2309.0
156.00	2653.0
157.00	499.0
158.00	729.0
159.00	488.0
159.90	1088.0
161.00	1767.0
162.00	301.0
164.90	1400.0
165.90	988.0
167.00	9871.0
168.00	5009.0
169.00	627.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

172.00	785.0
173.00	849.0
174.00	1790.0
175.00	3160.0
176.00	582.0
176.90	1483.0
178.00	453.0
179.00	6027.0
180.00	4057.0
180.90	1681.0
183.90	543.0
185.00	2708.0
186.00	20096.0
187.00	5967.0
187.90	674.0
188.90	1664.0
191.00	747.0
192.00	1918.0
193.00	2427.0
194.00	518.0
196.00	3193.0
196.90	632.0
197.90	108832.0
198.90	8121.0
200.00	791.0
201.40	424.0
202.90	1304.0
204.00	5718.0
205.00	9489.0
206.00	37624.0
207.00	6001.0
208.00	1704.0
209.10	601.0
209.90	651.0
211.00	1711.0
214.80	528.0
215.90	994.0
216.90	11587.0
218.00	1633.0
220.90	3563.0
221.90	1684.0
222.90	2471.0
224.00	23288.0
225.00	5833.0
226.00	670.0
227.00	11460.0
228.00	1761.0
228.90	2005.0
231.00	905.0
233.90	738.0
235.00	659.0
236.00	674.0
237.00	804.0
239.00	449.0
240.00	371.0
241.00	510.0
241.90	1193.0
242.90	1495.0
244.00	16289.0
245.00	2106.0
246.00	4468.0
246.90	702.0
248.90	545.0
253.10	556.0
254.10	704.0
255.00	89280.0
256.00	13547.0
256.90	957.0
258.00	6688.0
258.90	1255.0
265.00	3082.0
265.90	424.0
271.90	484.0
273.00	2596.0
274.00	6905.0
275.00	35568.0
276.00	4566.0
276.90	4760.0
278.00	761.0
282.90	529.0
284.00	354.0
284.90	717.0
293.00	731.0
294.90	304.0
296.00	15880.0
297.00	1750.0
303.00	1406.0
303.90	448.0
314.00	659.0
314.90	1777.0
315.90	654.0
320.90	380.0
323.00	3537.0
324.00	624.0
327.00	876.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

328.00	491.0
332.00	473.0
332.90	440.0
334.00	2444.0
335.00	613.0
341.00	418.0
345.90	1136.0
352.00	979.0
353.00	900.0
354.00	1115.0
355.00	305.0
365.00	7793.0
366.00	1112.0
372.00	1999.0
372.90	479.0
383.00	493.0
402.00	670.0
403.00	881.0
404.10	330.0
421.00	599.0
422.00	604.0
423.00	5139.0
424.00	1209.0
441.00	12317.0
442.00	77344.0
443.00	15504.0
444.00	1525.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
38.00	470.0
39.10	2150.0
39.90	304.0
43.90	778.0
50.10	8682.0
51.10	29128.0
52.00	1359.0
55.90	970.0
56.90	1774.0
61.00	337.0
62.00	423.0
63.00	1327.0
65.00	526.0
68.00	475.0
69.00	29416.0
73.10	809.0
74.10	3706.0
75.00	5533.0
76.10	1704.0
77.00	34992.0
78.00	2146.0
79.00	2585.0
80.00	2189.0
81.00	2842.0
82.00	601.0
82.90	476.0
85.00	425.0
86.00	981.0
87.00	337.0
91.00	708.0
92.00	734.0
93.00	5178.0
94.00	356.0
98.00	4276.0
99.00	2996.0
101.00	1456.0
103.00	334.0
104.00	900.0
104.90	984.0
106.10	320.0
107.00	12121.0
108.00	1533.0
109.00	364.0
110.00	17544.0
111.00	2960.0
111.90	397.0
116.00	684.0
117.00	16952.0
118.00	1131.0
121.90	883.0
123.00	1668.0
123.90	505.0
125.00	591.0
127.00	37248.0
128.00	2744.0
129.00	15503.0
129.90	1286.0
133.90	438.0
135.00	1352.0
135.90	522.0
136.90	884.0
140.90	2360.0
142.00	770.0
143.00	609.0
146.00	583.0
147.00	1644.0
147.90	4059.0
148.90	857.0
153.00	749.0
153.90	743.0
155.00	1288.0
156.00	1857.0
157.80	426.0
158.90	404.0
160.00	886.0
161.00	1427.0
164.90	1110.0
165.90	975.0
167.00	6952.0
168.00	3535.0
168.90	390.0
170.90	321.0
171.90	571.0
173.00	727.0
174.00	1380.0
175.00	2172.0
176.00	413.0
177.00	877.0
178.90	4047.0
180.00	2616.0
181.00	1375.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

184.00	329.0
185.00	1985.0
186.00	14543.0
187.00	4107.0
188.00	554.0
189.00	1308.0
191.00	765.0
192.00	1440.0
193.00	1678.0
193.90	304.0
196.00	2414.0
197.00	529.0
197.90	80440.0
199.00	5220.0
200.00	587.0
201.50	325.0
202.90	838.0
204.00	4170.0
205.00	7128.0
206.00	26656.0
207.00	4323.0
208.00	1300.0
208.90	548.0
209.90	586.0
211.00	1338.0
214.90	453.0
215.90	707.0
217.00	9403.0
217.90	1161.0
221.00	2773.0
221.90	1023.0
223.00	1983.0
224.00	17552.0
225.00	3805.0
226.00	488.0
227.00	8279.0
227.90	1197.0
228.90	1697.0
231.00	839.0
233.90	437.0
234.90	500.0
235.90	444.0
237.00	595.0
238.90	462.0
240.90	430.0
242.00	1044.0
242.90	809.0
244.00	12608.0
245.00	1664.0
246.00	3263.0
246.90	692.0
248.90	515.0
252.90	366.0
254.20	448.0
255.00	69536.0
256.00	9368.0
257.00	830.0
258.00	5336.0
259.00	865.0
264.90	2394.0
265.80	364.0
273.00	1900.0
274.00	5323.0
275.00	27952.0
276.00	3561.0
277.00	3324.0
277.90	649.0
282.90	476.0
283.90	323.0
284.90	503.0
292.90	883.0
296.00	12221.0
297.00	1545.0
302.90	1209.0
304.00	411.0
314.10	406.0
314.90	1460.0
316.00	664.0
320.90	410.0
323.00	3291.0
324.00	570.0
326.90	734.0
327.90	391.0
332.90	378.0
334.00	2371.0
335.00	564.0
340.90	319.0
346.00	752.0
352.00	1061.0
352.90	822.0
354.00	1014.0
365.00	6667.0
366.00	1054.0
370.90	302.0
372.00	1948.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

373.00	390.0
382.90	436.0
402.00	666.0
403.00	671.0
404.00	341.0
420.90	686.0
422.00	677.0
423.00	4029.0
424.00	1089.0
441.00	11343.0
442.00	72824.0
443.10	12751.0
444.00	1019.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

Scan 2454 (17.421 min): BM021890.D
DFTPP01

m/z	Abundance
40.00	312.0
44.00	608.0
206.90	829.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01