




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047118.D
Acq On : 09 Aug 2024 12:56
Operator : RC/JU
Sample : P3435-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X7

Manual IntegrationsAPPROVED

Quant Time: Aug 09 13:38:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:30:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :mohammad ahmed 08/12/2024

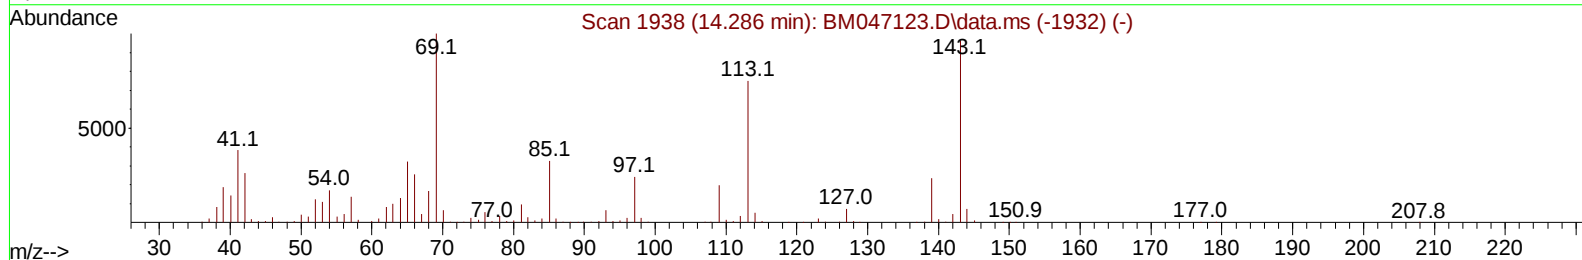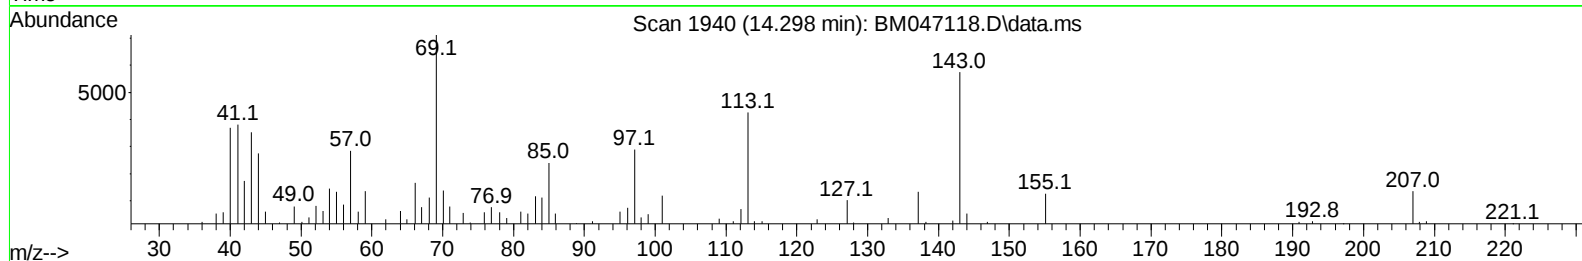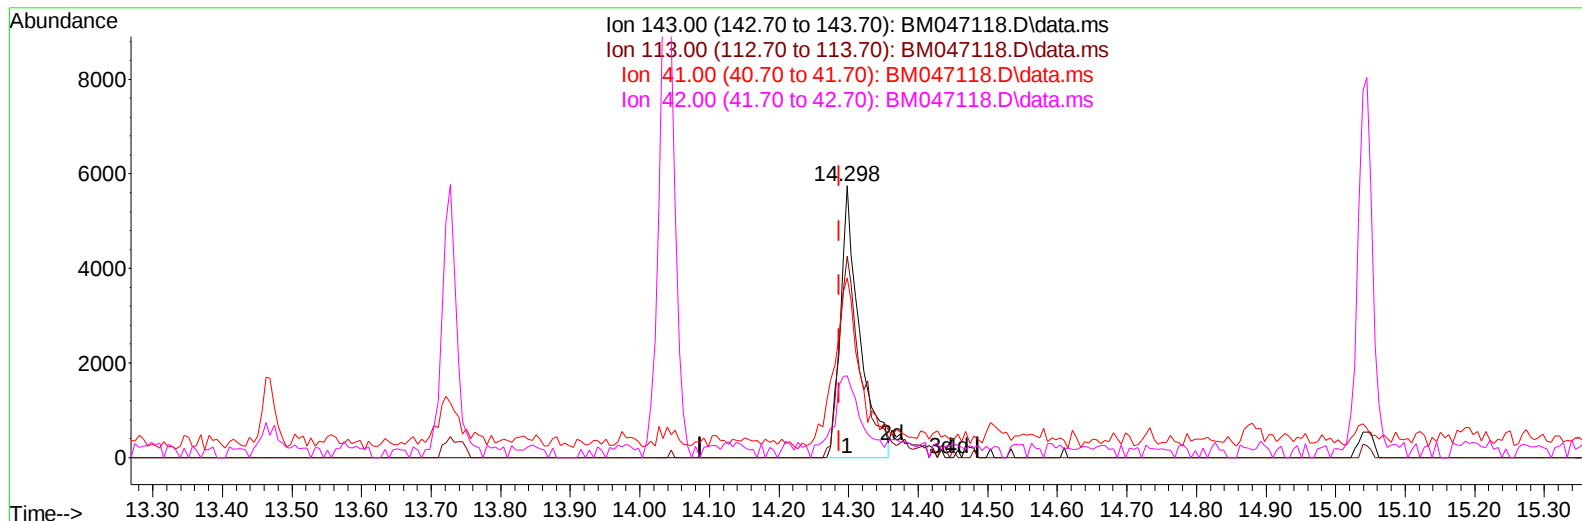

TIC: BM047118.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.298min (+ 0.012) 1.16 ng/u1

response 11018

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.30	74.09#
41.00	41.40	66.23#
42.00	29.30	30.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047118.D
Acq On : 09 Aug 2024 12:56
Operator : RC/JU
Sample : P3435-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :mohammad ahmed 08/12/2024

Quant Time: Aug 09 13:38:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:30:34 2024
Response via : Initial Calibration

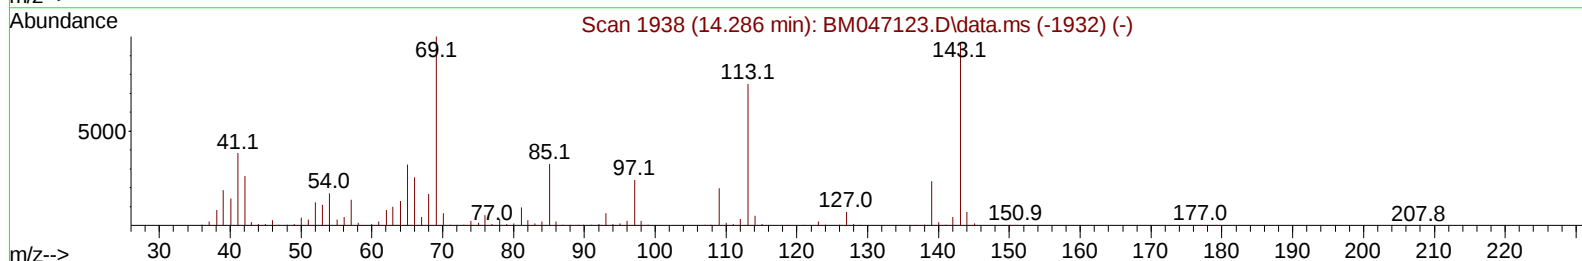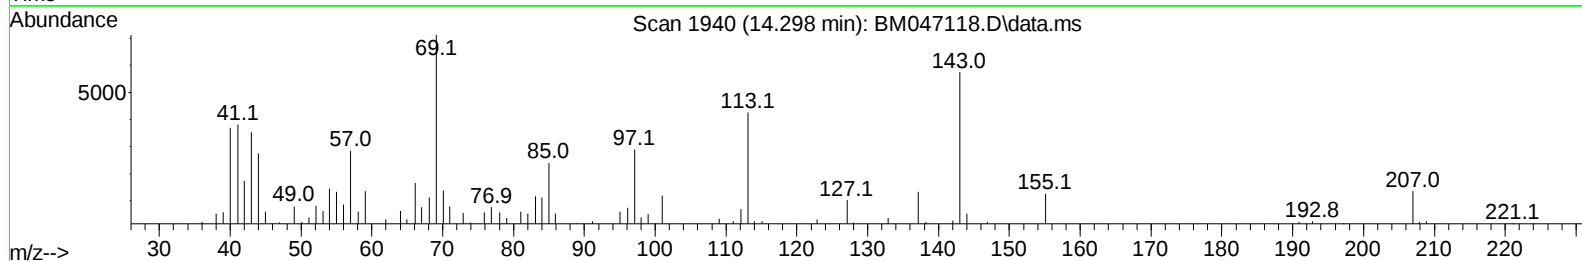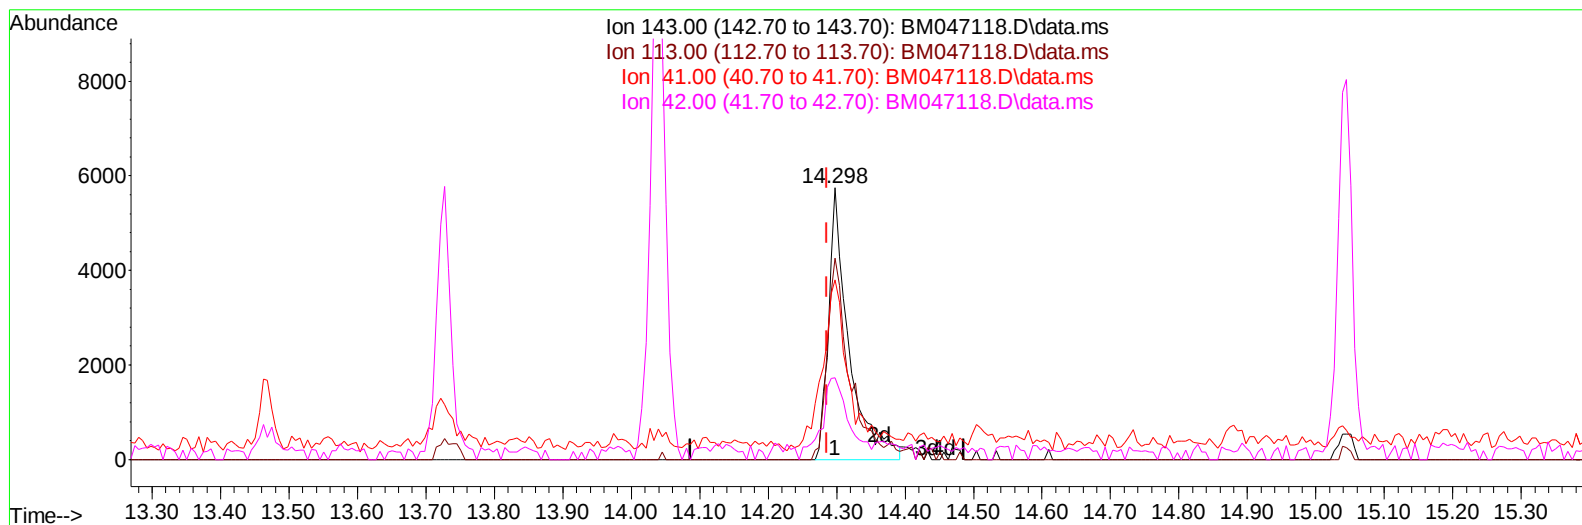

TIC: BM047118.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.298min (+ 0.012) 1.25 ng/ul m

response 11854

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.30	74.09#
41.00	41.40	66.23#
42.00	29.30	30.15

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047118.D
 Acq On : 09 Aug 2024 12:56
 Operator : RC/JU
 Sample : P3435-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E05X7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/12/2024
 Supervised By :mohammad ahmed 08/12/2024

Quant Time: Aug 10 01:05:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 01:30:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.387	152	257216	20.000	ng/ul	0.00
20) Naphthalene-d8	10.139	136	1024771	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.039	164	640068	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.798	188	1303027	20.000	ng/ul	0.00
79) Chrysene-d12	21.033	240	1113645	20.000	ng/ul	# 0.00
88) Perylene-d12	23.738	264	1320875	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.016	96	11867	1.828	ng/uL	0.00
4) Pyridine-d5	3.404	84	132599	7.488	ng/ul	0.00
7) Phenol-d5	6.593	99	250852	12.838	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.745	67	163435	12.712	ng/ul	0.00
11) 2-Chlorophenol-d4	6.928	132	187758	11.344	ng/ul	0.00
15) 4-Methylphenol-d8	8.104	113	198919	12.851	ng/ul	0.00
21) Nitrobenzene-d5	8.528	128	97383	11.843	ng/ul	0.00
24) 2-Nitrophenol-d4	9.239	143	87036	9.692	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.781	165	172710	10.017	ng/ul	0.00
31) 4-Chloroaniline-d4	10.292	131	233307	10.296	ng/ul	0.00
46) Dimethylphthalate-d6	13.469	166	563553	11.515	ng/ul	0.00
49) Acenaphthylene-d8	13.727	160	674848	12.353	ng/ul	0.00
54) 4-Nitrophenol-d4	14.298	143	11854m	1.253	ng/ul	0.01
60) Fluorene-d10	15.045	176	495063	11.825	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.186	200	6799	0.826	ng/ul	0.00
73) Anthracene-d10	16.898	188	746725	12.088	ng/ul	0.00
81) Pyrene-d10	19.209	212	833533	13.075	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.550	264	846077	12.164	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047118.D
Acq On : 09 Aug 2024 12:56
Operator : RC/JU
Sample : P3435-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :mohammad ahmed 08/12/2024

Quant Time: Aug 10 01:05:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:30:34 2024
Response via : Initial Calibration

