

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047107.D
 Acq On : 09 Aug 2024 05:31
 Operator : RC/JU
 Sample : P3434-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E05W9

Quant Time: Aug 09 06:18:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 01:30:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.387	152	244089	20.000	ng/u1	0.00
20) Naphthalene-d8	10.139	136	963418	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.039	164	608162	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.798	188	1237557	20.000	ng/u1	0.00
79) Chrysene-d12	21.033	240	1070902	20.000	ng/u1	# 0.00
88) Perylene-d12	23.733	264	1031402	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.016	96	25364	4.117	ng/uL	0.00
4) Pyridine-d5	3.405	84	403815	24.029	ng/u1	0.00
7) Phenol-d5	6.593	99	556536	30.015	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.745	67	342242	28.052	ng/u1	0.00
11) 2-Chlorophenol-d4	6.928	132	441756	28.125	ng/u1	0.00
15) 4-Methylphenol-d8	8.104	113	428295	29.158	ng/u1	0.00
21) Nitrobenzene-d5	8.528	128	220686	28.546	ng/u1	0.00
24) 2-Nitrophenol-d4	9.239	143	252896	29.955	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.781	165	460177	28.390	ng/u1	0.00
31) 4-Chloroaniline-d4	10.292	131	395858	18.582	ng/u1	0.00
46) Dimethylphthalate-d6	13.469	166	1317220	28.327	ng/u1	0.00
49) Acenaphthylene-d8	13.727	160	1491936	28.743	ng/u1	0.00
54) 4-Nitrophenol-d4	14.286	143	186038	20.692	ng/u1	0.00
60) Fluorene-d10	15.045	176	1140692	28.676	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.186	200	135331	17.308	ng/u1	0.00
73) Anthracene-d10	16.898	188	1255286	21.396	ng/u1	0.00
81) Pyrene-d10	19.215	212	1855786	30.272	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.550	264	1276417	23.502	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.616	94	20520	1.099	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047107.D
Acq On : 09 Aug 2024 05:31
Operator : RC/JU
Sample : P3434-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05W9

Quant Time: Aug 09 06:18:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:30:34 2024
Response via : Initial Calibration

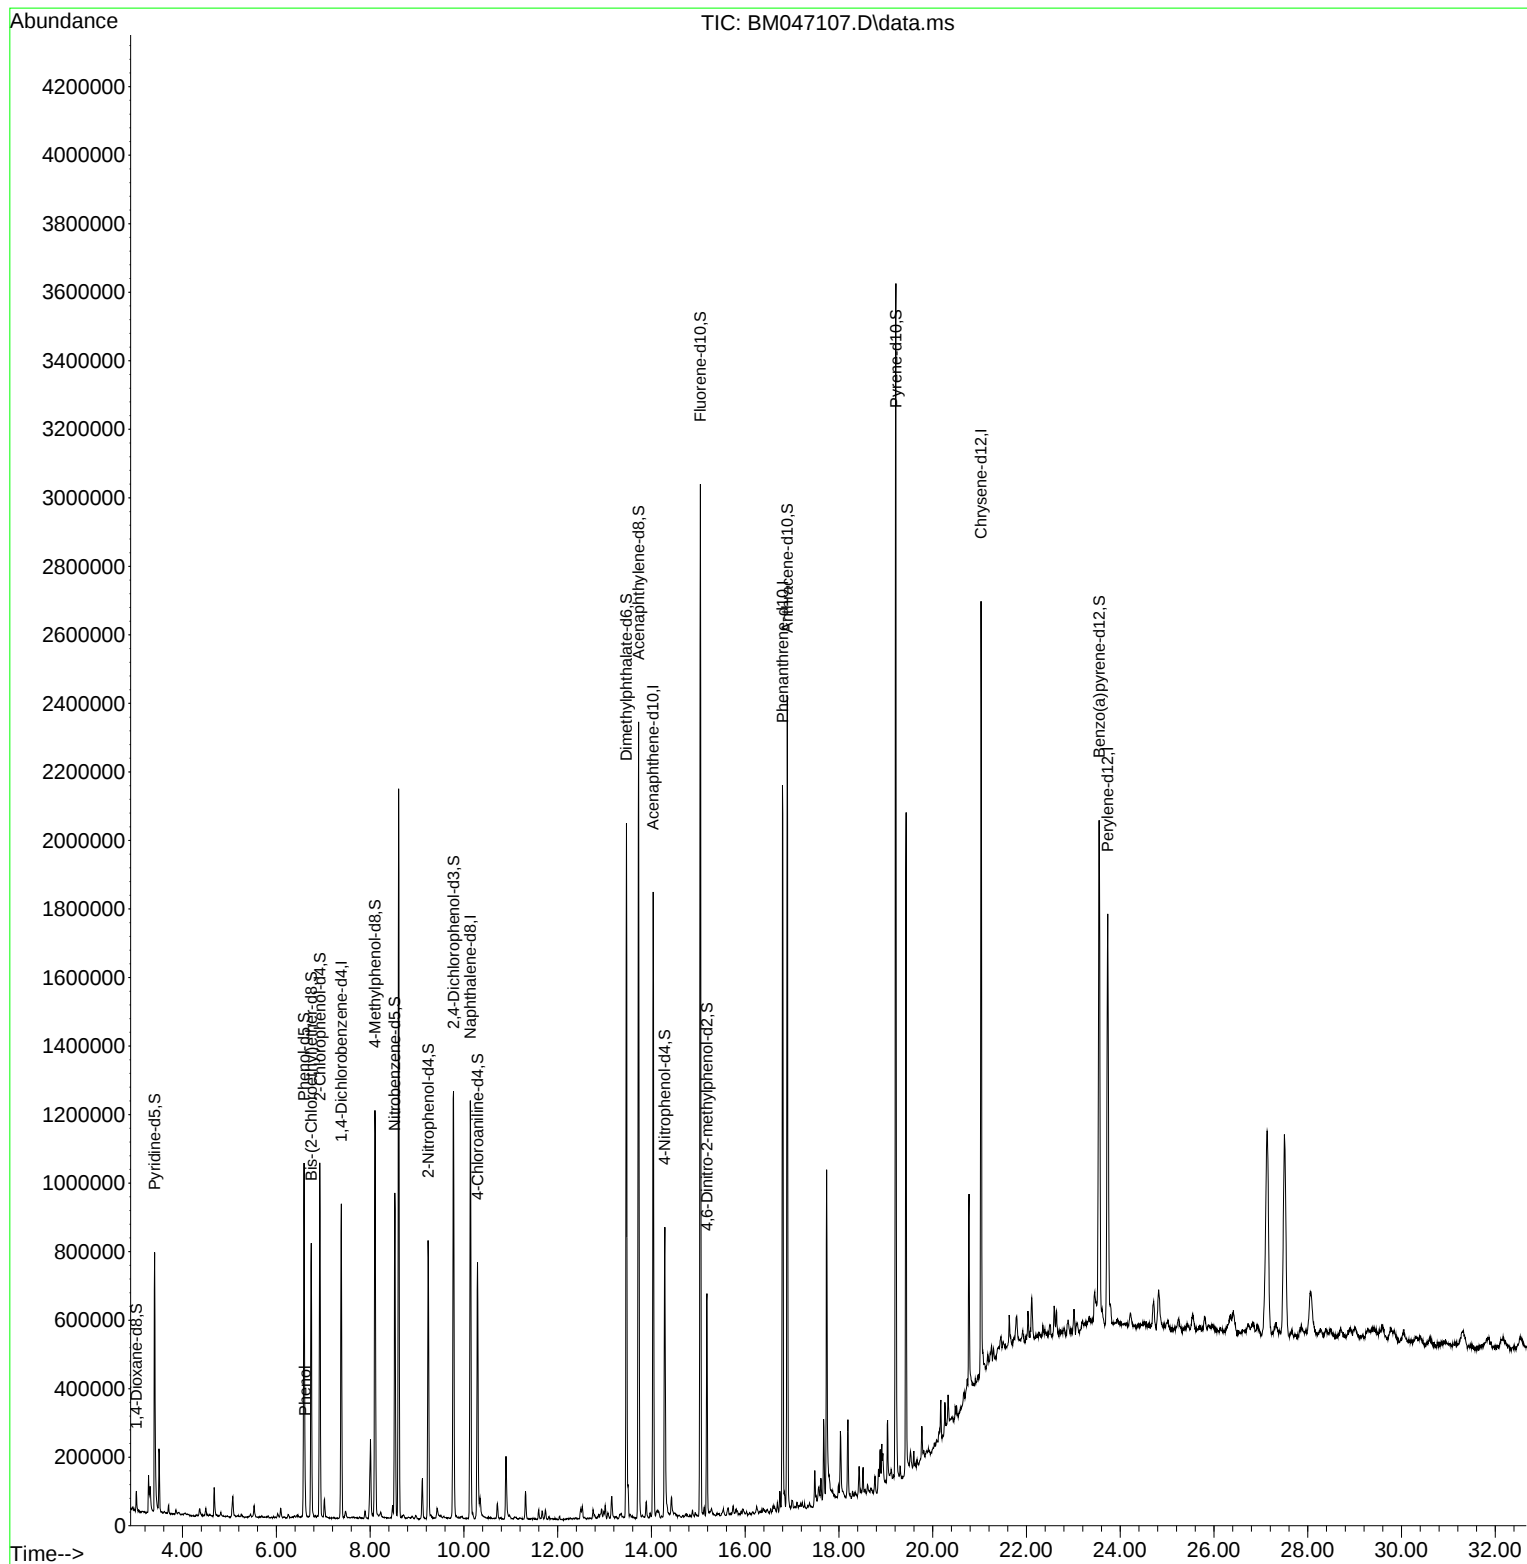

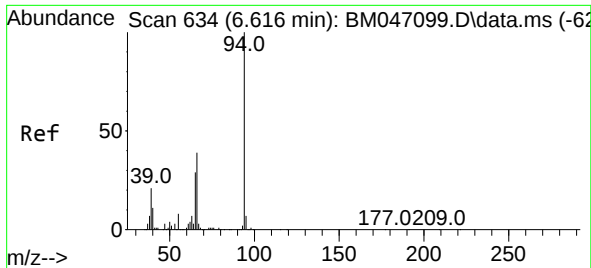

Phenol
 Concen: 1.099 ng/ul
 RT: 6.616 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM047107.D
 Acq: 09 Aug 2024 05:31

Instrument :
 BNA_M
 ClientSampleId :
 E05W9

Tgt Ion: 94 Resp: 20520
 Ion Ratio Lower Upper
 94 100
 65 33.6 25.1 37.7
 66 52.4 37.7 56.5

