

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047094.D
 Acq On : 08 Aug 2024 20:07
 Operator : RC/JU
 Sample : P3435-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E05X3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	19	22	30	rVB	35320	49996	1.45%	0.132%
2	3.287	66	68	75	rBV2	8614	10956	0.32%	0.029%
3	3.404	85	88	106	rBV	401637	576354	16.68%	1.519%
4	3.704	135	139	143	rVB	19359	26283	0.76%	0.069%
5	5.081	371	373	377	rBV5	3128	3645	0.11%	0.010%
6	6.445	604	605	607	rBV2	3775	3643	0.11%	0.010%
7	6.593	624	630	640	rVB	512684	772284	22.35%	2.035%
8	6.745	650	656	665	rVB	415429	616236	17.84%	1.624%
9	6.928	681	687	697	rBV	531497	805558	23.31%	2.123%
10	7.263	742	744	748	rBV6	2727	3788	0.11%	0.010%
11	7.387	758	765	775	rBV	1072081	1611822	46.65%	4.248%
12	8.104	881	887	901	rBV	613994	954858	27.64%	2.516%
13	8.304	918	921	924	rVB3	2442	3665	0.11%	0.010%
14	8.528	952	959	969	rBV	464443	760842	22.02%	2.005%
15	8.722	991	992	998	rVB5	2580	3804	0.11%	0.010%
16	9.122	1056	1060	1066	rVB7	6291	9829	0.28%	0.026%
17	9.245	1073	1081	1089	rBV	370823	616213	17.83%	1.624%
18	9.304	1089	1091	1096	rVB5	3548	5270	0.15%	0.014%
19	9.681	1151	1155	1159	rVB6	1819	3706	0.11%	0.010%
20	9.781	1164	1172	1188	rBV	592819	1004651	29.08%	2.648%
21	10.139	1226	1233	1245	rBV	1358065	2228768	64.51%	5.873%
22	10.292	1252	1259	1272	rBV	588376	974318	28.20%	2.568%
23	10.475	1285	1290	1291	rVB4	3140	3656	0.11%	0.010%
24	10.728	1331	1333	1338	rVB4	4980	6571	0.19%	0.017%
25	10.904	1357	1363	1370	rBV	36502	70423	2.04%	0.186%
26	10.975	1373	1375	1384	rVB9	4637	10292	0.30%	0.027%
27	11.275	1422	1426	1429	rVV6	3264	5107	0.15%	0.013%
28	11.675	1491	1494	1496	rBV4	4682	4563	0.13%	0.012%
29	11.745	1500	1506	1511	rVB4	12089	22974	0.66%	0.061%
30	12.045	1552	1557	1561	rVB5	4941	7982	0.23%	0.021%
31	12.133	1566	1572	1574	rBV6	2181	3774	0.11%	0.010%
32	12.386	1609	1615	1619	rBV5	4610	9445	0.27%	0.025%
33	12.645	1656	1659	1664	rVB4	5022	6915	0.20%	0.018%
34	13.116	1737	1739	1743	rBV5	3438	3526	0.10%	0.009%
35	13.304	1766	1771	1773	rVB4	2869	4206	0.12%	0.011%
36	13.469	1793	1799	1810	rBV	1025341	1367002	39.56%	3.602%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047094.D
Acq On : 08 Aug 2024 20:07
Operator : RC/JU
Sample : P3435-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	13.727	1836	1843	1855	rBV	1167949	1715501	49.65%	4.521%
38	14.039	1889	1896	1904	rBV	1993923	2919826	84.51%	7.694%
39	14.286	1929	1938	1957	rBV2	278103	565328	16.36%	1.490%
40	14.510	1973	1976	1982	rVV8	6902	10413	0.30%	0.027%
41	14.580	1986	1988	1991	rVB4	3817	4362	0.13%	0.011%
42	14.821	2025	2029	2032	rVV6	3669	5663	0.16%	0.015%
43	14.880	2034	2039	2047	rBV7	7094	13078	0.38%	0.034%
44	15.045	2060	2067	2076	rBV	1501809	2108499	61.03%	5.556%
45	15.186	2085	2091	2099	rBV	239891	348245	10.08%	0.918%
46	15.286	2102	2108	2114	rVB10	7136	15149	0.44%	0.040%
47	15.615	2158	2164	2165	rBV4	2776	4508	0.13%	0.012%
48	15.639	2165	2168	2170	rVB4	3123	4107	0.12%	0.011%
49	15.733	2180	2184	2189	rVB5	6105	9236	0.27%	0.024%
50	15.868	2205	2207	2211	rVB5	2655	3788	0.11%	0.010%
51	15.968	2218	2224	2227	rBV7	3836	6630	0.19%	0.017%
52	16.051	2236	2238	2243	rVB6	2481	3910	0.11%	0.010%
53	16.457	2305	2307	2309	rBV3	3177	3463	0.10%	0.009%
54	16.598	2324	2331	2335	rBV7	7344	18408	0.53%	0.049%
55	16.798	2356	2365	2372	rBV	2456574	3381520	97.87%	8.911%
56	16.898	2376	2382	2396	rVB	1604891	2183086	63.18%	5.753%
57	17.021	2401	2403	2407	rVB5	10401	10768	0.31%	0.028%
58	17.515	2485	2487	2491	rVB5	7104	6313	0.18%	0.017%
59	17.615	2501	2504	2506	rVV4	4044	4947	0.14%	0.013%
60	17.739	2520	2525	2532	rBV	148823	227424	6.58%	0.599%
61	18.039	2573	2576	2579	rVB5	7881	10308	0.30%	0.027%
62	18.680	2682	2685	2687	rBV4	7479	8933	0.26%	0.024%
63	18.774	2697	2701	2704	rBV5	17552	23922	0.69%	0.063%
64	18.851	2710	2714	2717	rBV	15994	23097	0.67%	0.061%
65	19.039	2741	2746	2753	rBV2	105758	164582	4.76%	0.434%
66	19.209	2770	2775	2784	rBV	1758502	2425276	70.19%	6.391%
67	20.774	3039	3041	3047	rVB3	57520	63618	1.84%	0.168%
68	21.033	3080	3085	3094	rBV	2507157	3360846	97.27%	8.857%
69	23.550	3506	3513	3523	rVB	1072369	2264335	65.54%	5.967%
70	23.733	3537	3544	3553	rBV	1536486	3455115	100.00%	9.105%




Sum of corrected areas: 37947129

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047094.D
Acq On : 08 Aug 2024 20:07
Operator : RC/JU
Sample : P3435-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

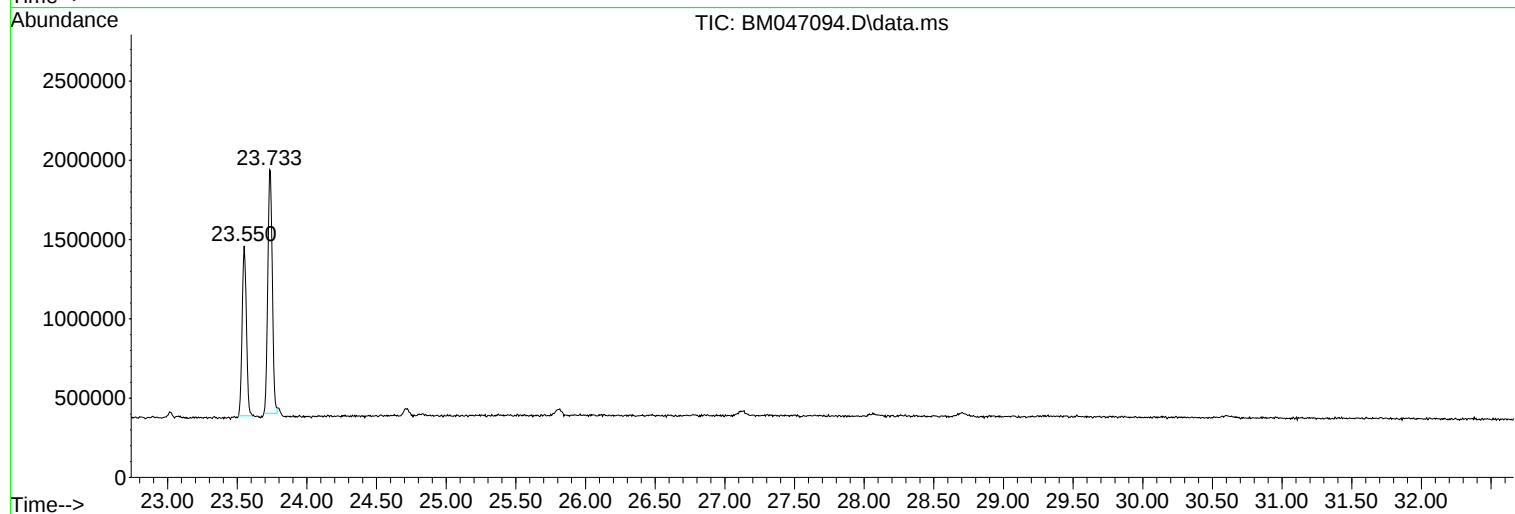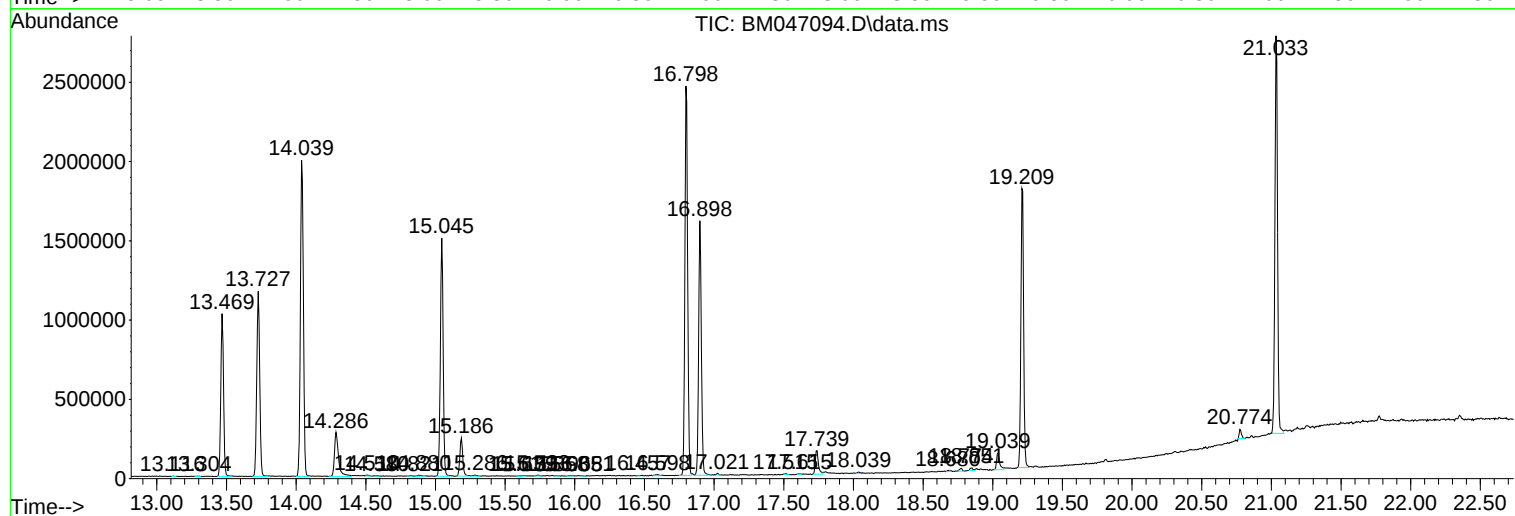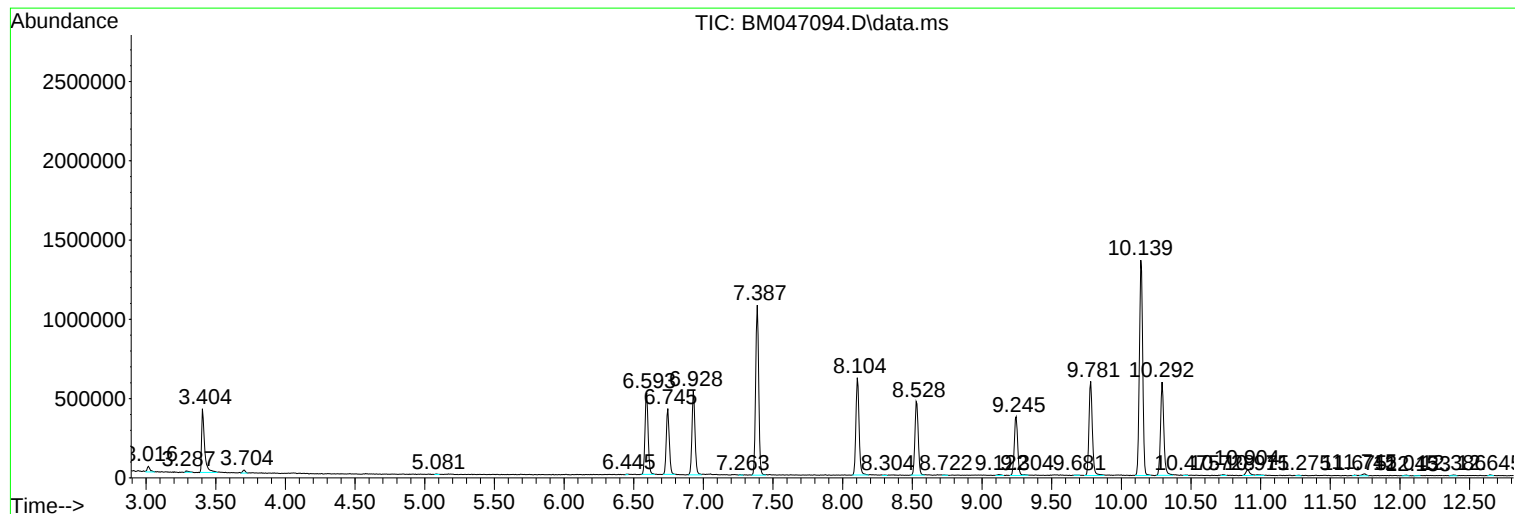

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047094.D
Acq On : 08 Aug 2024 20:07
Operator : RC/JU
Sample : P3435-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047094.D
Acq On : 08 Aug 2024 20:07
Operator : RC/JU
Sample : P3435-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E05X3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc