

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047111.D
 Acq On : 09 Aug 2024 08:11
 Operator : RC/JU
 Sample : P3435-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0600

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	20	23	25	rVB2	10959	10121	0.29%	0.039%
2	3.410	86	89	103	rBV	109649	172649	5.02%	0.657%
3	3.698	135	138	143	rVB	21107	27659	0.80%	0.105%
4	4.004	189	190	194	rBV4	4304	5146	0.15%	0.020%
5	4.687	305	306	311	rBV5	2362	3444	0.10%	0.013%
6	4.922	343	346	349	rBV5	3217	4564	0.13%	0.017%
7	5.192	389	392	394	rVB3	3542	3977	0.12%	0.015%
8	6.339	581	587	589	rBV7	1970	3993	0.12%	0.015%
9	6.445	602	605	607	rBV4	2737	3700	0.11%	0.014%
10	6.592	624	630	640	rBV	204269	329706	9.59%	1.255%
11	6.745	650	656	663	rVB	167883	253343	7.37%	0.965%
12	6.928	681	687	694	rBV	216545	332335	9.66%	1.265%
13	7.386	757	765	775	rBV	1017412	1540766	44.80%	5.866%
14	8.004	865	870	871	rBV5	4193	5402	0.16%	0.021%
15	8.104	881	887	895	rBV	259192	421843	12.27%	1.606%
16	8.375	930	933	935	rVB4	2975	3630	0.11%	0.014%
17	8.398	935	937	940	rBV4	2871	4200	0.12%	0.016%
18	8.528	953	959	968	rVV	201682	333180	9.69%	1.269%
19	8.716	988	991	996	rVB7	3861	4411	0.13%	0.017%
20	8.969	1032	1034	1038	rVB5	3888	5418	0.16%	0.021%
21	9.116	1054	1059	1064	rBV3	23120	39611	1.15%	0.151%
22	9.245	1074	1081	1089	rBV	154961	258130	7.51%	0.983%
23	9.522	1123	1128	1136	rVB10	6790	16417	0.48%	0.063%
24	9.780	1162	1172	1180	rBV	265076	454660	13.22%	1.731%
25	10.139	1225	1233	1248	rBV	1295965	2136169	62.11%	8.133%
26	10.292	1251	1259	1270	rBV	259338	452096	13.15%	1.721%
27	10.722	1328	1332	1336	rBV5	7148	9863	0.29%	0.038%
28	10.904	1356	1363	1372	rBV2	43011	92636	2.69%	0.353%
29	10.974	1372	1375	1379	rVB6	4537	6796	0.20%	0.026%
30	11.386	1440	1445	1447	rBV6	1952	3821	0.11%	0.015%
31	11.745	1501	1506	1512	rVB7	6330	10098	0.29%	0.038%
32	12.721	1669	1672	1675	rVB5	2897	3814	0.11%	0.015%
33	13.468	1792	1799	1810	rBV	509985	695973	20.24%	2.650%
34	13.727	1833	1843	1854	rBV	586889	848036	24.66%	3.229%
35	13.804	1854	1856	1861	rBV6	3491	4873	0.14%	0.019%
36	13.974	1880	1885	1887	rBV5	3091	4838	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047111.D
 Acq On : 09 Aug 2024 08:11
 Operator : RC/JU
 Sample : P3435-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0600

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	14.039	1889	1896	1903	rBV	1950591	2750770	79.98%	10.474%
38	14.221	1922	1927	1930	rVB6	3086	3810	0.11%	0.015%
39	14.298	1930	1940	1948	rBV3	50180	116039	3.37%	0.442%
40	14.868	2034	2037	2041	rVB5	3350	4669	0.14%	0.018%
41	14.939	2046	2049	2051	rVV4	4307	5127	0.15%	0.020%
42	15.045	2061	2067	2080	rVB	747777	1055904	30.70%	4.020%
43	15.186	2084	2091	2097	rBV	32834	52848	1.54%	0.201%
44	15.286	2104	2108	2112	rBV7	3727	5846	0.17%	0.022%
45	15.451	2133	2136	2141	rVB7	2750	4527	0.13%	0.017%
46	15.498	2141	2144	2147	rBV5	3288	4470	0.13%	0.017%
47	15.621	2161	2165	2167	rBV4	4444	5409	0.16%	0.021%
48	15.733	2180	2184	2190	rVB9	5204	8780	0.26%	0.033%
49	15.804	2192	2196	2199	rVV6	4184	6466	0.19%	0.025%
50	15.839	2199	2202	2209	rVB7	2720	5716	0.17%	0.022%
51	16.256	2268	2273	2277	rBV6	4428	6282	0.18%	0.024%
52	16.556	2319	2324	2326	rBV6	4249	6912	0.20%	0.026%
53	16.592	2326	2330	2334	rVV6	8377	13841	0.40%	0.053%
54	16.662	2339	2342	2347	rBV7	4792	7861	0.23%	0.030%
55	16.798	2359	2365	2376	rBV	2255204	3164407	92.01%	12.049%
56	16.898	2376	2382	2395	rVB	792162	1139409	33.13%	4.338%
57	17.127	2416	2421	2422	rBV5	3904	3991	0.12%	0.015%
58	17.574	2493	2497	2499	rBV5	2960	3696	0.11%	0.014%
59	17.609	2499	2503	2505	rBV5	8237	13470	0.39%	0.051%
60	17.733	2520	2524	2531	rBV2	77670	113927	3.31%	0.434%
61	17.998	2567	2569	2572	rBV4	4033	4779	0.14%	0.018%
62	18.039	2572	2576	2577	rBV4	8720	10258	0.30%	0.039%
63	18.345	2626	2628	2629	rBV2	4731	3795	0.11%	0.014%
64	18.768	2697	2700	2705	rBV7	11633	16270	0.47%	0.062%
65	19.033	2742	2745	2750	rBV7	30293	42528	1.24%	0.162%
66	19.209	2769	2775	2783	rBV	977323	1303214	37.89%	4.962%
67	20.774	3039	3041	3046	rVB2	85422	90846	2.64%	0.346%
68	21.033	3080	3085	3091	rBV	2368326	3108272	90.38%	11.835%
69	23.550	3507	3513	3524	rVB	603729	1233197	35.86%	4.695%
70	23.732	3537	3544	3561	rVB	1420740	3439201	100.00%	13.095%




Sum of corrected areas: 26263855

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047111.D
Acq On : 09 Aug 2024 08:11
Operator : RC/JU
Sample : P3435-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0600

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

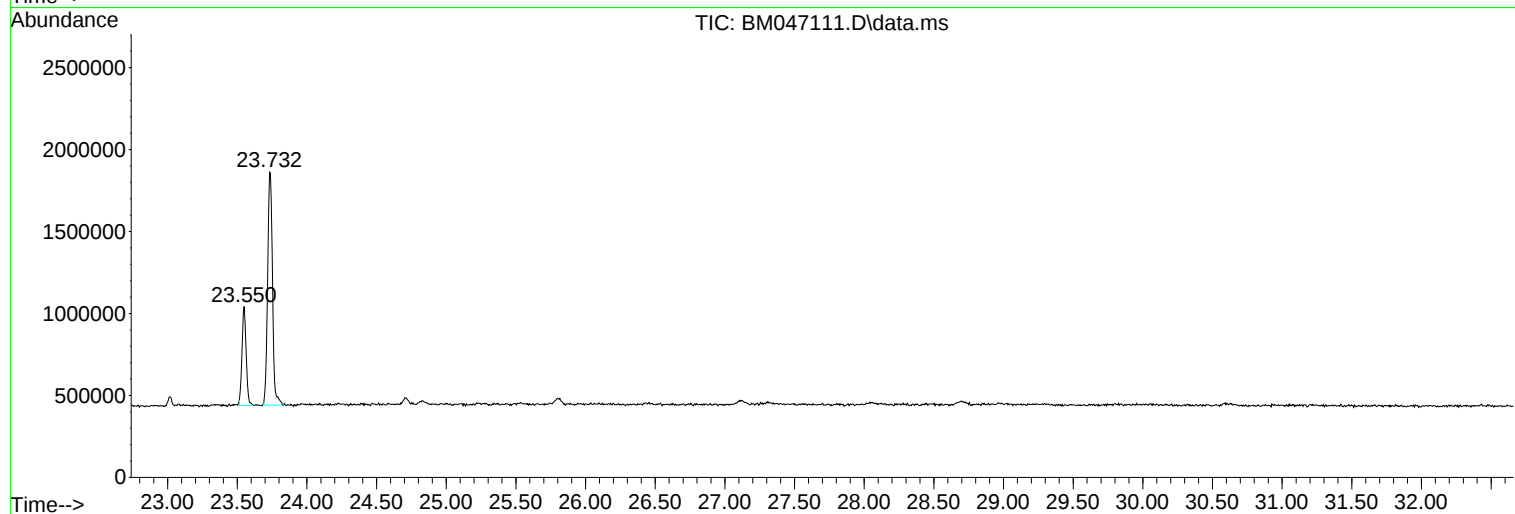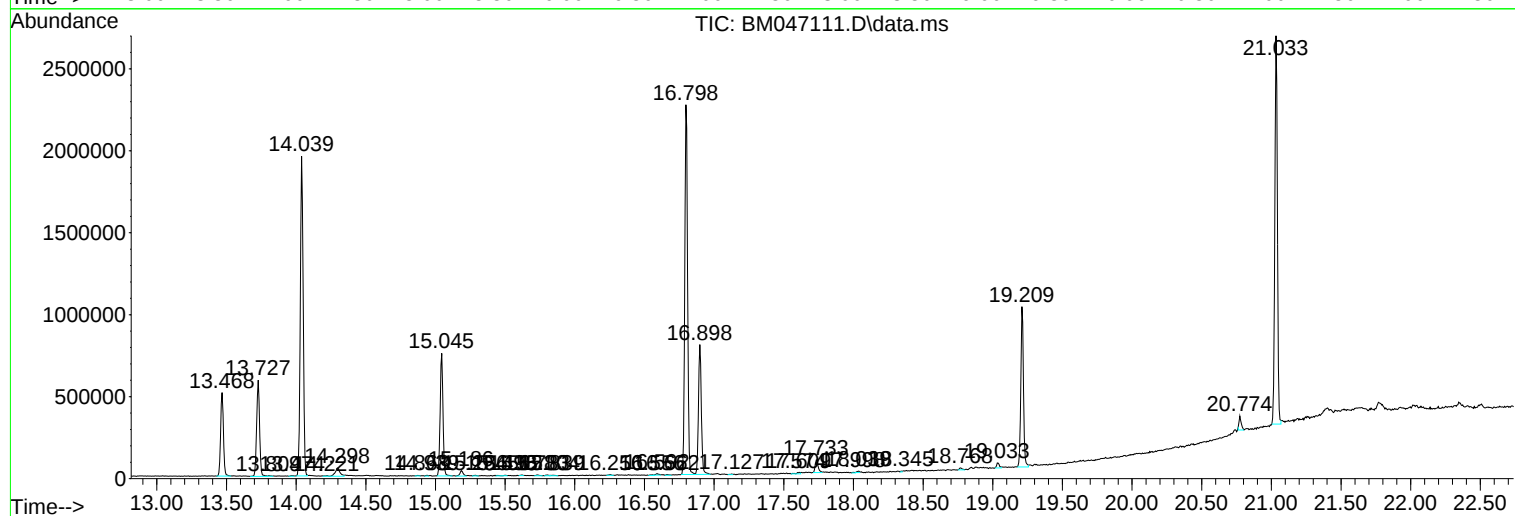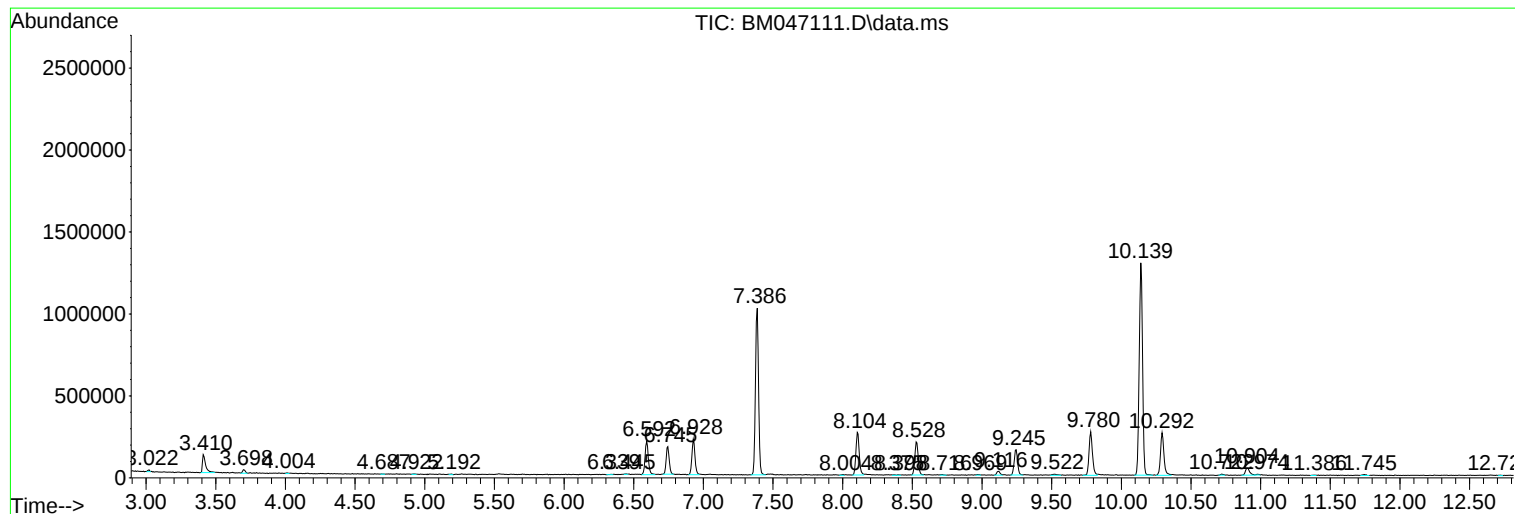

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047111.D
Acq On : 09 Aug 2024 08:11
Operator : RC/JU
Sample : P3435-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0600

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047111.D
Acq On : 09 Aug 2024 08:11
Operator : RC/JU
Sample : P3435-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0600

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc