

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047124.D
 Acq On : 09 Aug 2024 17:01
 Operator : RC/JU
 Sample : PB162595BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK595

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	18	22	27	rBV	68727	84470	1.96%	0.172%
2	3.404	84	88	107	rBV	800132	1181946	27.48%	2.408%
3	3.575	115	117	119	rBV3	4364	4493	0.10%	0.009%
4	3.698	134	138	145	rVB	18716	24259	0.56%	0.049%
5	6.592	623	630	639	rBV	975651	1478938	34.38%	3.013%
6	6.745	650	656	670	rVB	755111	1159130	26.95%	2.362%
7	6.928	680	687	702	rBV	961341	1470074	34.18%	2.995%
8	7.386	758	765	774	rVB	706963	1110450	25.82%	2.262%
9	8.104	881	887	900	rBV	1117247	1778903	41.36%	3.624%
10	8.528	952	959	970	rBV	914516	1429964	33.25%	2.913%
11	9.239	1072	1080	1090	rBV	738537	1193442	27.75%	2.431%
12	9.339	1095	1097	1102	rVB6	3006	4467	0.10%	0.009%
13	9.780	1165	1172	1190	rBV	1112737	1855743	43.15%	3.781%
14	9.898	1190	1192	1197	rVB6	3081	4729	0.11%	0.010%
15	10.139	1225	1233	1242	rBV	960104	1542715	35.87%	3.143%
16	10.292	1252	1259	1272	rBV	1091680	1828815	42.52%	3.726%
17	11.745	1500	1506	1511	rBV2	16113	31242	0.73%	0.064%
18	11.969	1540	1544	1548	rBV5	3360	6269	0.15%	0.013%
19	12.998	1715	1719	1727	rVB10	4511	8926	0.21%	0.018%
20	13.468	1793	1799	1809	rBV	1762543	2444032	56.82%	4.979%
21	13.727	1836	1843	1854	rBV	2065223	3052077	70.96%	6.218%
22	14.039	1889	1896	1904	rBV	1393025	1995479	46.39%	4.065%
23	14.174	1912	1919	1920	rBV6	3374	5817	0.14%	0.012%
24	14.286	1931	1938	1955	rBV	814519	1322539	30.75%	2.694%
25	14.727	2009	2013	2016	rBV5	3593	4451	0.10%	0.009%
26	15.045	2060	2067	2080	rBV	2673175	3675717	85.46%	7.489%
27	15.186	2085	2091	2099	rBV	779551	1044726	24.29%	2.128%
28	15.292	2104	2109	2115	rVB5	12810	21055	0.49%	0.043%
29	15.609	2158	2163	2164	rBV5	5024	4813	0.11%	0.010%
30	15.833	2198	2201	2207	rVB5	8737	11824	0.27%	0.024%
31	16.309	2278	2282	2284	rVB5	3223	4762	0.11%	0.010%
32	16.798	2359	2365	2375	rBV	1628475	2274045	52.87%	4.633%
33	16.898	2375	2382	2396	rBV2	2740795	3904098	90.77%	7.954%
34	17.739	2522	2525	2533	rBV7	8919	14754	0.34%	0.030%
35	17.803	2533	2536	2539	rBV5	5221	4818	0.11%	0.010%
36	18.727	2691	2693	2695	rBV3	5967	4392	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047124.D
Acq On : 09 Aug 2024 17:01
Operator : RC/JU
Sample : PB162595BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	18.774	2697	2701	2706	rVV3	36868	51533	1.20%	0.105%
38	18.845	2709	2713	2718	rBV	32688	44746	1.04%	0.091%
39	19.215	2769	2776	2784	rBV	3108925	4301169	100.00%	8.763%
40	21.033	3080	3085	3091	rBV	1730473	2244619	52.19%	4.573%
41	23.556	3506	3514	3528	rVB2	1971030	4241692	98.62%	8.642%
42	23.732	3538	3544	3552	rBV	1001230	2211180	51.41%	4.505%




Sum of corrected areas: 49083313

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047124.D
Acq On : 09 Aug 2024 17:01
Operator : RC/JU
Sample : PB162595BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

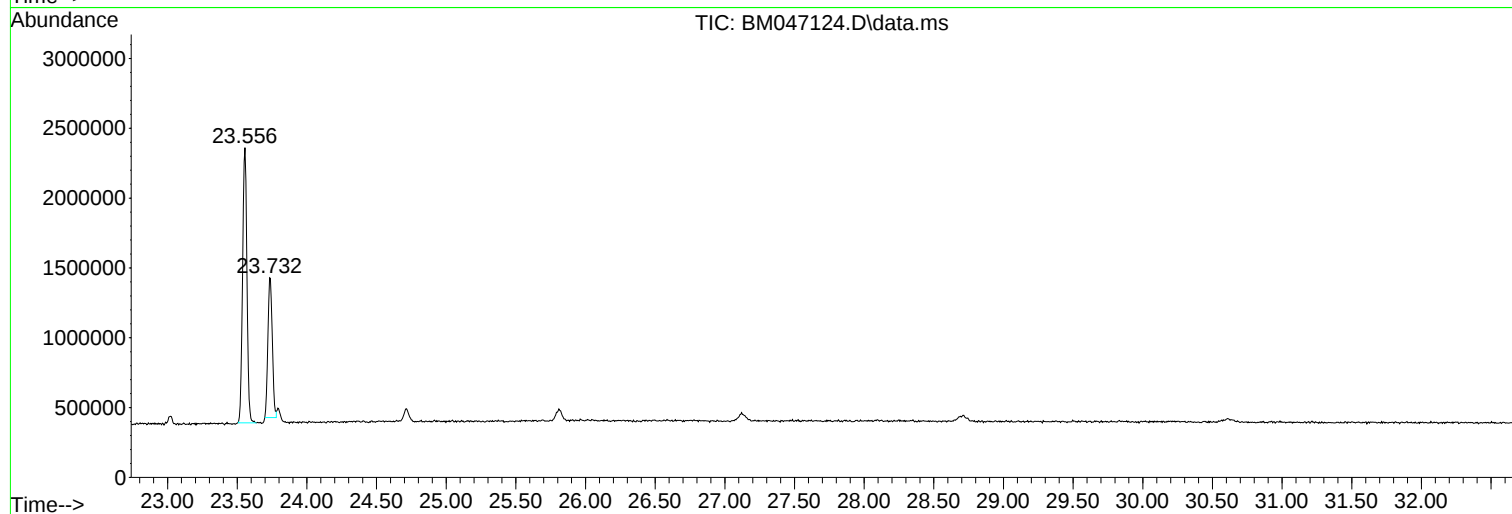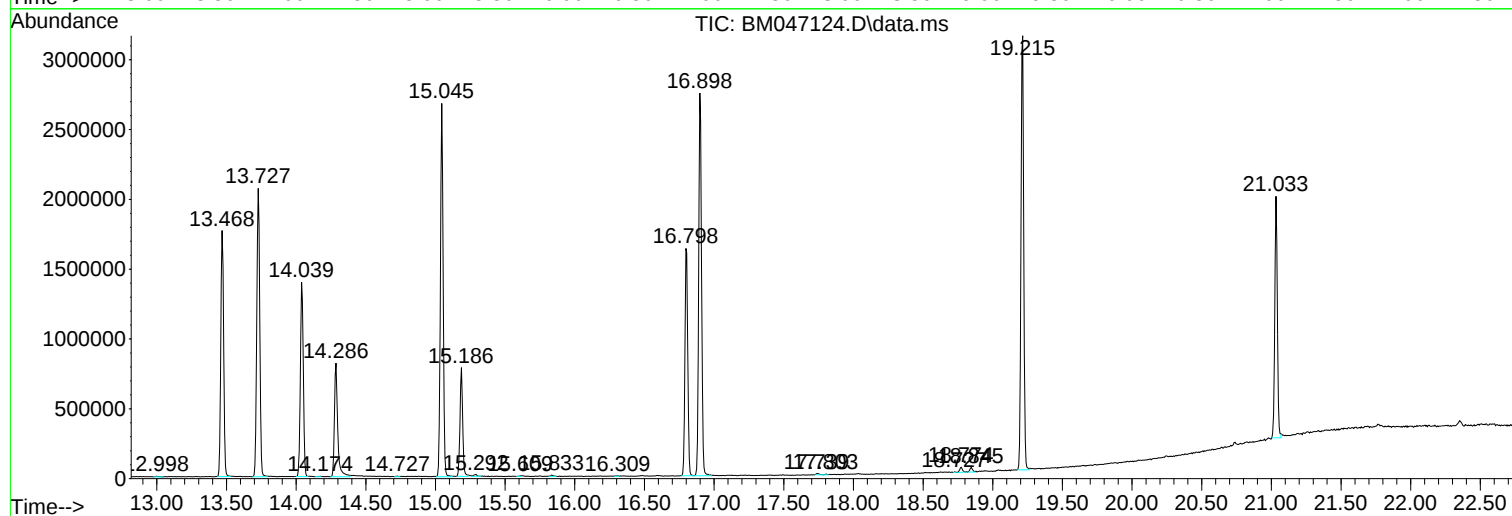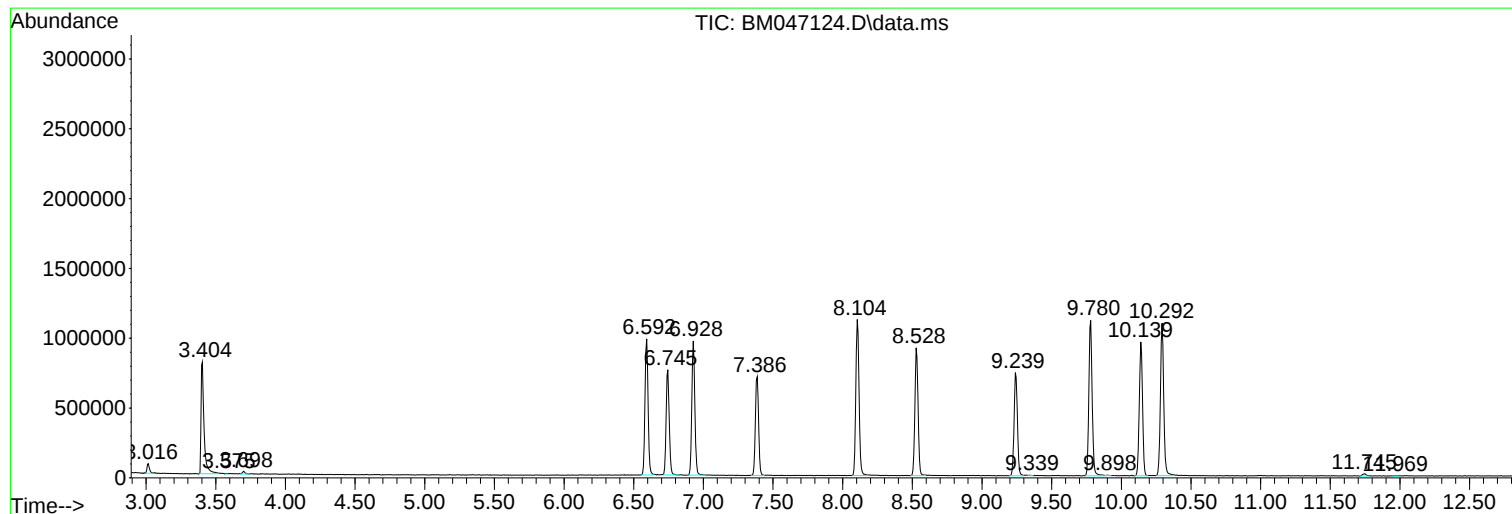

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047124.D
Acq On : 09 Aug 2024 17:01
Operator : RC/JU
Sample : PB162595BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047124.D
Acq On : 09 Aug 2024 17:01
Operator : RC/JU
Sample : PB162595BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc