

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047125.D
 Acq On : 09 Aug 2024 17:42
 Operator : RC/JU
 Sample : PB162619BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	18	22	34	rVB	66385	90083	2.23%	0.184%
2	3.399	84	87	106	rBV	769974	1132721	28.08%	2.313%
3	3.705	135	139	143	rVB2	16911	21580	0.53%	0.044%
4	4.893	338	341	344	rVB5	2627	4042	0.10%	0.008%
5	6.593	623	630	645	rBV	922464	1421809	35.25%	2.903%
6	6.746	650	656	666	rVB	703679	1091051	27.05%	2.228%
7	6.928	681	687	696	rBV	933529	1386083	34.36%	2.831%
8	7.387	757	765	772	rBV	833804	1302074	32.28%	2.659%
9	8.104	881	887	898	rBV	1092042	1667406	41.33%	3.405%
10	8.528	951	959	968	rBV	860138	1366834	33.88%	2.791%
11	8.981	1034	1036	1041	rBV6	3430	4268	0.11%	0.009%
12	9.240	1074	1080	1093	rBV	696559	1127584	27.95%	2.303%
13	9.687	1151	1156	1159	rBV6	2808	4607	0.11%	0.009%
14	9.775	1164	1171	1186	rVV	1015941	1741340	43.17%	3.556%
15	9.869	1186	1187	1191	rVB4	4709	5728	0.14%	0.012%
16	10.139	1225	1233	1245	rVB	1093792	1794871	44.49%	3.665%
17	10.292	1252	1259	1272	rBV	1019604	1735047	43.01%	3.543%
18	11.739	1501	1505	1512	rVB2	14174	25039	0.62%	0.051%
19	11.957	1538	1542	1546	rBV5	2127	4671	0.12%	0.010%
20	13.469	1793	1799	1811	rBV	1717262	2273901	56.37%	4.644%
21	13.727	1836	1843	1857	rBV	1938120	2812610	69.72%	5.744%
22	14.039	1889	1896	1906	rBV	1572637	2299061	56.99%	4.695%
23	14.286	1931	1938	1956	rBV	750178	1269683	31.47%	2.593%
24	14.469	1966	1969	1973	rVB6	3678	4163	0.10%	0.009%
25	15.045	2060	2067	2081	rBV	2413846	3396661	84.20%	6.936%
26	15.186	2085	2091	2101	rVV	731252	992965	24.61%	2.028%
27	15.286	2104	2108	2115	rVB5	11039	20250	0.50%	0.041%
28	15.616	2159	2164	2169	rVB7	5078	7283	0.18%	0.015%
29	15.833	2199	2201	2206	rVB6	7855	10483	0.26%	0.021%
30	16.798	2359	2365	2375	rBV	1875825	2639695	65.44%	5.391%
31	16.898	2376	2382	2392	rBV	2603586	3625475	89.87%	7.404%
32	17.115	2412	2419	2423	rBV10	4120	8389	0.21%	0.017%
33	17.192	2429	2432	2434	rBV4	5163	4453	0.11%	0.009%
34	17.292	2444	2449	2451	rBV6	3573	4951	0.12%	0.010%
35	17.739	2520	2525	2528	rBV7	6316	11055	0.27%	0.023%
36	17.833	2536	2541	2543	rBV5	2049	4100	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047125.D
Acq On : 09 Aug 2024 17:42
Operator : RC/JU
Sample : PB162619BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	18.039	2572	2576	2581	rBV8	5273	11368	0.28%	0.023%
38	18.774	2697	2701	2708	rVB2	30615	41990	1.04%	0.086%
39	18.845	2709	2713	2717	rBV2	25771	37451	0.93%	0.076%
40	19.209	2769	2775	2784	rBV	2992314	4022162	99.71%	8.214%
41	21.033	3080	3085	3095	rBV	2021108	2634686	65.31%	5.380%
42	23.556	3506	3514	3523	rVB	1891357	4034005	100.00%	8.238%
43	23.739	3537	3545	3552	rBV	1301073	2875512	71.28%	5.872%




Sum of corrected areas: 48969190

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047125.D
Acq On : 09 Aug 2024 17:42
Operator : RC/JU
Sample : PB162619BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK619

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

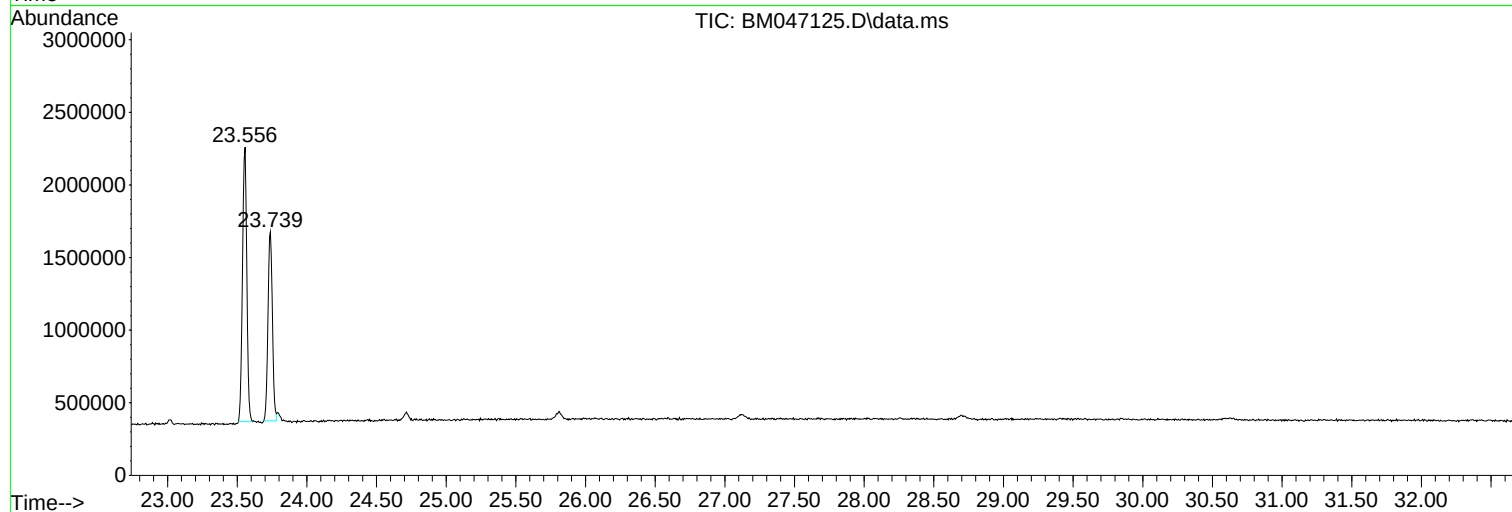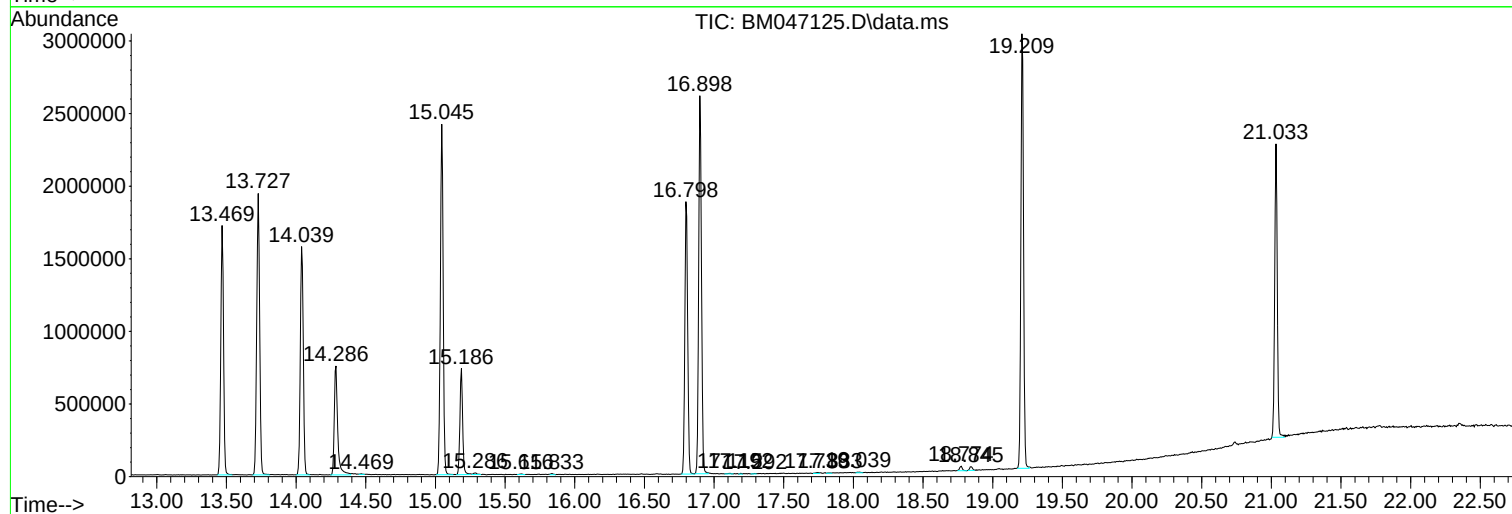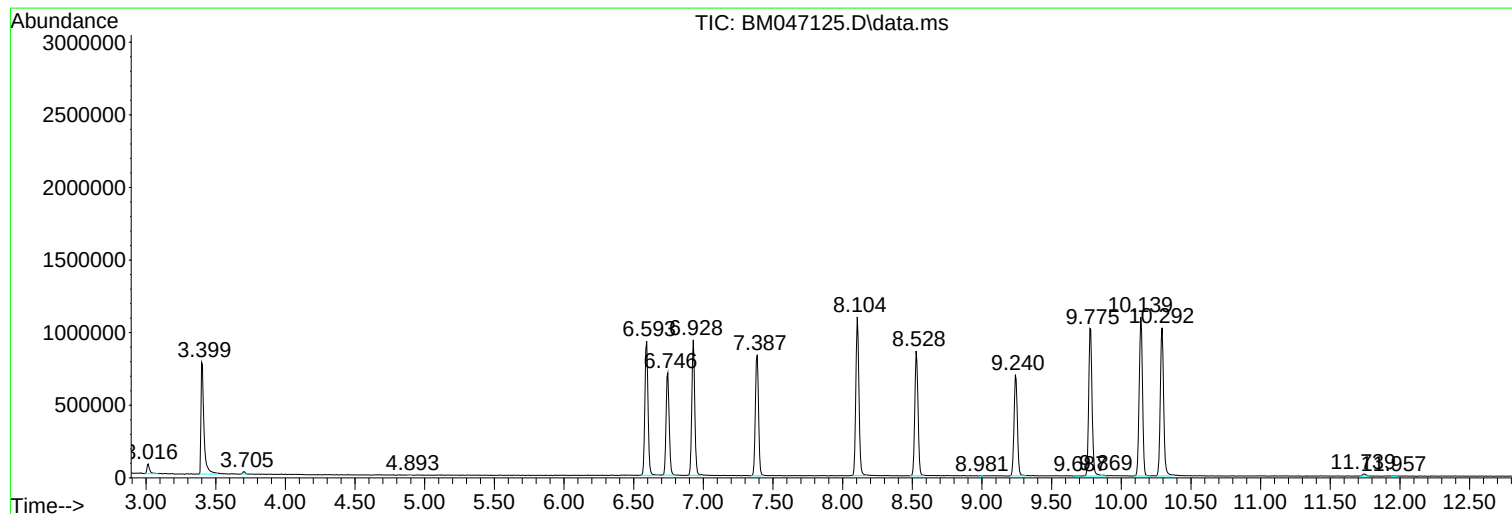

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047125.D
Acq On : 09 Aug 2024 17:42
Operator : RC/JU
Sample : PB162619BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK619

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047125.D
Acq On : 09 Aug 2024 17:42
Operator : RC/JU
Sample : PB162619BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK619

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc