

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047126.D
 Acq On : 09 Aug 2024 18:23
 Operator : RC/JU
 Sample : PB162597BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	17	22	27	rBV	66296	81581	2.00%	0.166%
2	3.398	84	87	107	rBV	784101	1152754	28.23%	2.343%
3	3.698	135	138	143	rVB	23193	29258	0.72%	0.059%
4	4.687	304	306	310	rBV5	3356	6025	0.15%	0.012%
5	6.592	622	630	641	rBV	938268	1438653	35.23%	2.923%
6	6.745	649	656	667	rVB	708518	1104267	27.04%	2.244%
7	6.928	679	687	698	rBV	934774	1429927	35.01%	2.906%
8	7.386	758	765	772	rBV	817663	1272347	31.15%	2.586%
9	8.104	881	887	896	rBV	1112006	1694927	41.50%	3.444%
10	8.204	903	904	912	rVB6	4591	6797	0.17%	0.014%
11	8.451	943	946	949	rBV5	3040	4448	0.11%	0.009%
12	8.528	952	959	968	rVV	862303	1380943	33.81%	2.806%
13	9.239	1073	1080	1092	rBV	719464	1150684	28.17%	2.338%
14	9.775	1164	1171	1183	rBV	1039053	1744362	42.71%	3.545%
15	10.139	1225	1233	1243	rVB	1097398	1758770	43.06%	3.574%
16	10.292	1249	1259	1271	rBV	1054739	1748744	42.82%	3.554%
17	10.986	1374	1377	1379	rBV3	3041	4268	0.10%	0.009%
18	11.745	1500	1506	1512	rBV3	14457	28312	0.69%	0.058%
19	13.468	1793	1799	1811	rBV	1704563	2311164	56.59%	4.697%
20	13.727	1836	1843	1853	rBV	1964295	2807720	68.75%	5.706%
21	14.039	1890	1896	1906	rBV	1530234	2233075	54.68%	4.538%
22	14.286	1931	1938	1953	rBV	774116	1286449	31.50%	2.614%
23	15.045	2060	2067	2079	rBV	2401579	3400429	83.26%	6.910%
24	15.186	2084	2091	2104	rBV	761190	1018506	24.94%	2.070%
25	15.280	2104	2107	2113	rVB6	11565	20410	0.50%	0.041%
26	15.615	2161	2164	2167	rVB5	4633	6410	0.16%	0.013%
27	15.839	2198	2202	2207	rVB5	6928	9563	0.23%	0.019%
28	16.168	2254	2258	2263	rVB6	3066	4851	0.12%	0.010%
29	16.586	2327	2329	2331	rBV3	3654	4217	0.10%	0.009%
30	16.798	2359	2365	2372	rBV	1875154	2582478	63.23%	5.248%
31	16.898	2376	2382	2395	rVV2	2618664	3680752	90.12%	7.480%
32	17.109	2413	2418	2419	rBV5	4967	7060	0.17%	0.014%
33	17.739	2522	2525	2529	rBV5	9225	13849	0.34%	0.028%
34	18.768	2697	2700	2707	rVB3	30699	43248	1.06%	0.088%
35	18.845	2709	2713	2717	rVV	30569	38613	0.95%	0.078%
36	19.209	2769	2775	2787	rBV	3017518	4059443	99.40%	8.249%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047126.D
Acq On : 09 Aug 2024 18:23
Operator : RC/JU
Sample : PB162597BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	21.033	3080	3085	3094	rBV	1976488	2605883	63.81%	5.295%
38	23.556	3506	3514	3523	rVB2	1911471	4084081	100.00%	8.299%
39	23.732	3537	3544	3561	rVB	1282125	2954998	72.35%	6.005%




Sum of corrected areas: 49210266

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047126.D
Acq On : 09 Aug 2024 18:23
Operator : RC/JU
Sample : PB162597BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

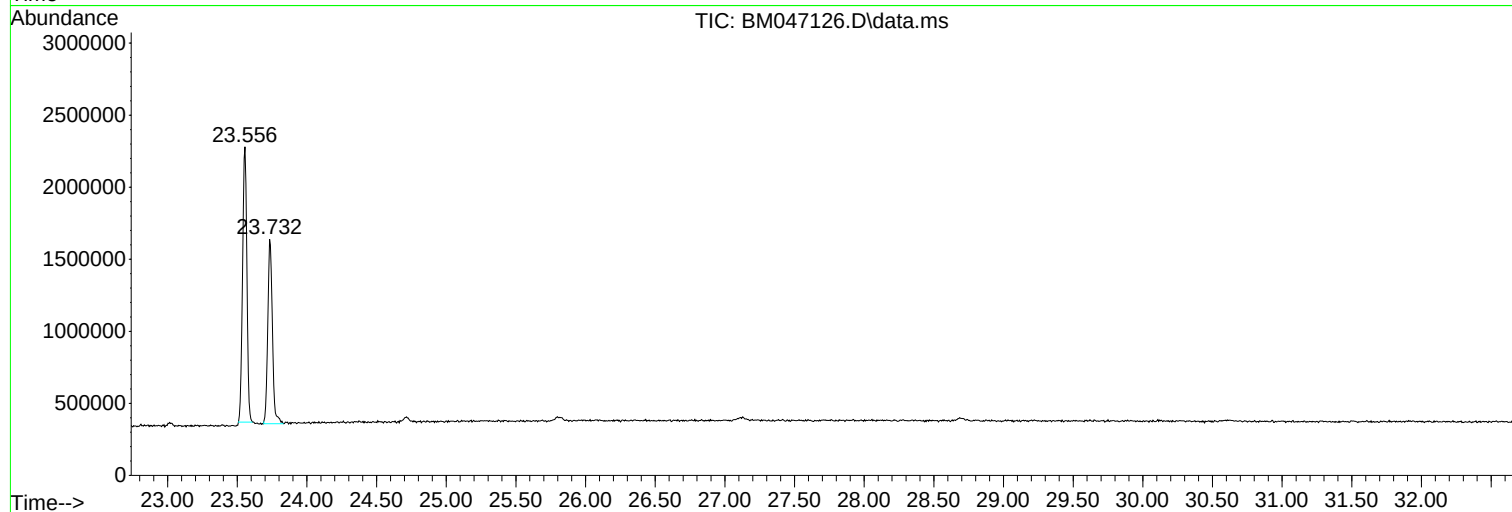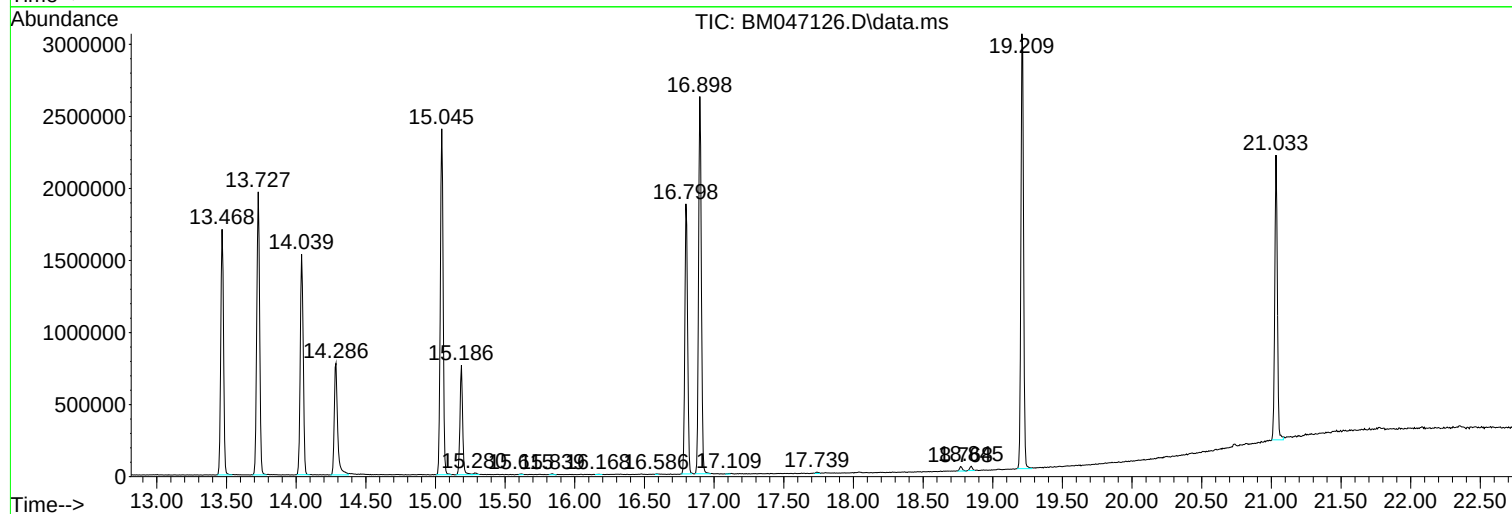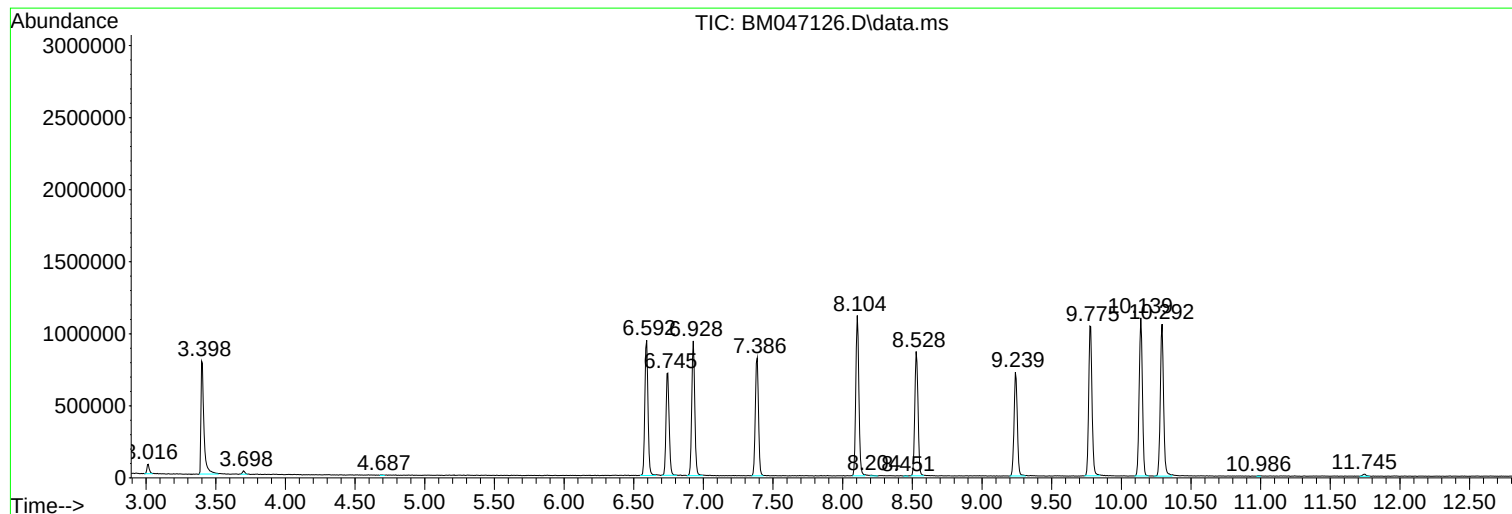

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047126.D
Acq On : 09 Aug 2024 18:23
Operator : RC/JU
Sample : PB162597BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047126.D
Acq On : 09 Aug 2024 18:23
Operator : RC/JU
Sample : PB162597BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc