

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047128.D
 Acq On : 09 Aug 2024 19:44
 Operator : RC/JU
 Sample : P3480-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	18	22	34	rVB	57794	82727	1.70%	0.169%
2	3.410	85	89	104	rBV	165633	264440	5.44%	0.541%
3	3.699	135	138	143	rVB	26446	32137	0.66%	0.066%
4	4.575	284	287	292	rBV7	6354	10273	0.21%	0.021%
5	5.687	473	476	480	rBV6	5164	6660	0.14%	0.014%
6	6.593	623	630	641	rVB	199589	318244	6.54%	0.651%
7	6.740	649	655	665	rBV	670503	1026927	21.11%	2.102%
8	6.928	680	687	696	rBV	737677	1138022	23.40%	2.329%
9	7.028	702	704	710	rVB7	5689	9106	0.19%	0.019%
10	7.381	758	764	772	rBV	901611	1424569	29.29%	2.915%
11	8.104	880	887	897	rBV	580267	913495	18.78%	1.869%
12	8.204	901	904	910	rVB4	11033	17115	0.35%	0.035%
13	8.528	952	959	970	rBV	835858	1303436	26.80%	2.667%
14	8.687	982	986	989	rBV5	3806	5667	0.12%	0.012%
15	9.239	1074	1080	1091	rBV	579681	930520	19.13%	1.904%
16	9.775	1165	1171	1184	rBV	928084	1556991	32.01%	3.186%
17	10.139	1225	1233	1246	rVB	1245768	2020819	41.54%	4.135%
18	10.292	1251	1259	1275	rBV	792343	1384877	28.47%	2.834%
19	10.792	1337	1344	1351	rBV6	13000	26235	0.54%	0.054%
20	11.675	1489	1494	1495	rBV5	3854	5759	0.12%	0.012%
21	11.739	1500	1505	1510	rVV2	19088	30974	0.64%	0.063%
22	12.039	1552	1556	1560	rVB6	3684	5340	0.11%	0.011%
23	12.386	1609	1615	1619	rBV8	6994	11634	0.24%	0.024%
24	12.645	1654	1659	1665	rVB4	12709	16976	0.35%	0.035%
25	13.039	1723	1726	1731	rVV6	4523	6704	0.14%	0.014%
26	13.469	1792	1799	1806	rBV	1624953	2252342	46.30%	4.609%
27	13.727	1836	1843	1852	rBV	1944272	2793737	57.43%	5.717%
28	14.039	1890	1896	1904	rBV	1845181	2653851	54.56%	5.431%
29	14.104	1904	1907	1916	rVB	7927	14604	0.30%	0.030%
30	14.286	1932	1938	1952	rBV	110927	232008	4.77%	0.475%
31	14.504	1971	1975	1977	rBV4	4296	4931	0.10%	0.010%
32	14.721	2009	2012	2016	rBV6	4963	6274	0.13%	0.013%
33	14.816	2024	2028	2033	rBV4	6645	9107	0.19%	0.019%
34	14.892	2033	2041	2045	rBV2	13508	28569	0.59%	0.058%
35	15.045	2060	2067	2083	rBV	2472558	3493081	71.81%	7.148%
36	15.186	2085	2091	2099	rVV	559538	779596	16.03%	1.595%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047128.D
 Acq On : 09 Aug 2024 19:44
 Operator : RC/JU
 Sample : P3480-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	15.286	2102	2108	2113	rVB5	12749	24984	0.51%	0.051%
38	15.427	2125	2132	2139	rBV4	13015	23248	0.48%	0.048%
39	15.610	2160	2163	2165	rBV3	6213	6858	0.14%	0.014%
40	15.827	2198	2200	2204	rVB5	4448	5317	0.11%	0.011%
41	16.304	2277	2281	2286	rBV8	2948	5183	0.11%	0.011%
42	16.586	2325	2329	2333	rBV6	7532	13790	0.28%	0.028%
43	16.798	2359	2365	2371	rBV	2340073	3124038	64.22%	6.393%
44	16.898	2376	2382	2396	rVV	3001488	4147361	85.26%	8.487%
45	17.115	2414	2419	2424	rVB	20899	26791	0.55%	0.055%
46	17.186	2427	2431	2432	rBV4	5730	5096	0.10%	0.010%
47	17.492	2479	2483	2492	rVB10	21290	30802	0.63%	0.063%
48	17.733	2520	2524	2530	rBV8	23073	35245	0.72%	0.072%
49	17.798	2533	2535	2538	rVB	11832	11389	0.23%	0.023%
50	18.039	2572	2576	2580	rBV7	8066	14160	0.29%	0.029%
51	18.192	2600	2602	2605	rVB4	6299	6826	0.14%	0.014%
52	18.768	2696	2700	2706	rVB4	34369	49866	1.03%	0.102%
53	18.839	2709	2712	2716	rBV	41400	53142	1.09%	0.109%
54	19.033	2742	2745	2746	rBV3	13354	12849	0.26%	0.026%
55	19.209	2766	2775	2785	rBV	3540295	4753694	97.73%	9.728%
56	21.033	3080	3085	3094	rBV	2366435	3183415	65.44%	6.515%
57	23.550	3505	3513	3523	rBV	2196887	4864300	100.00%	9.954%
58	23.733	3537	3544	3562	rVB	1565685	3649550	75.03%	7.469%




Sum of corrected areas: 48865651

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047128.D
Acq On : 09 Aug 2024 19:44
Operator : RC/JU
Sample : P3480-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

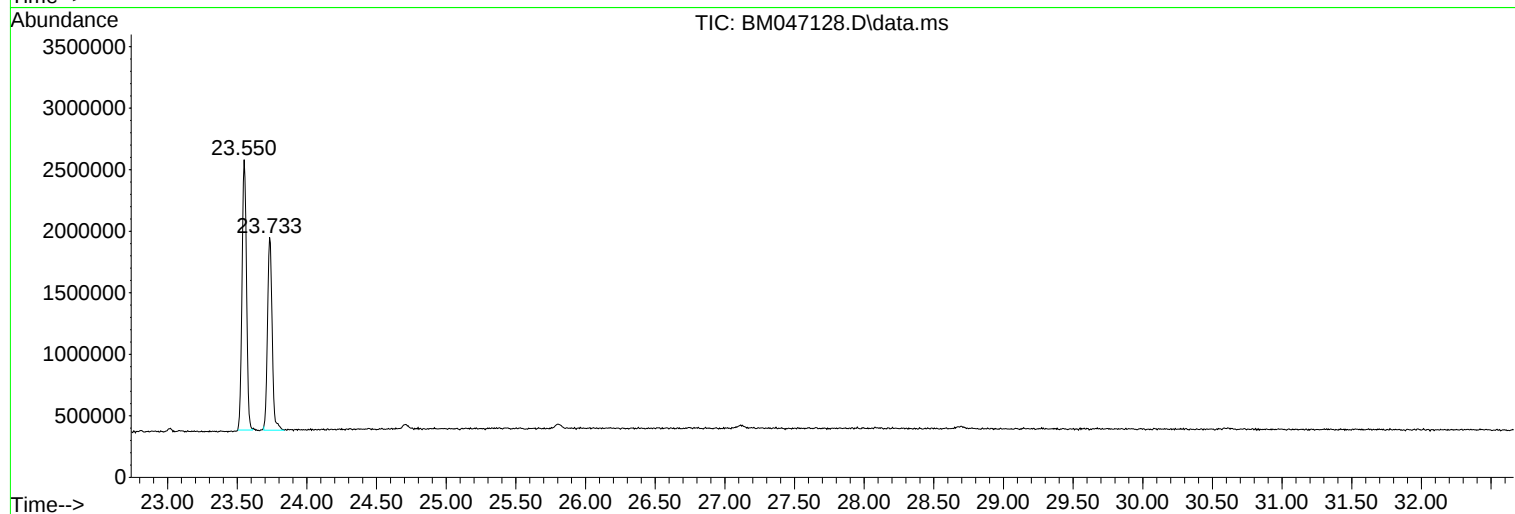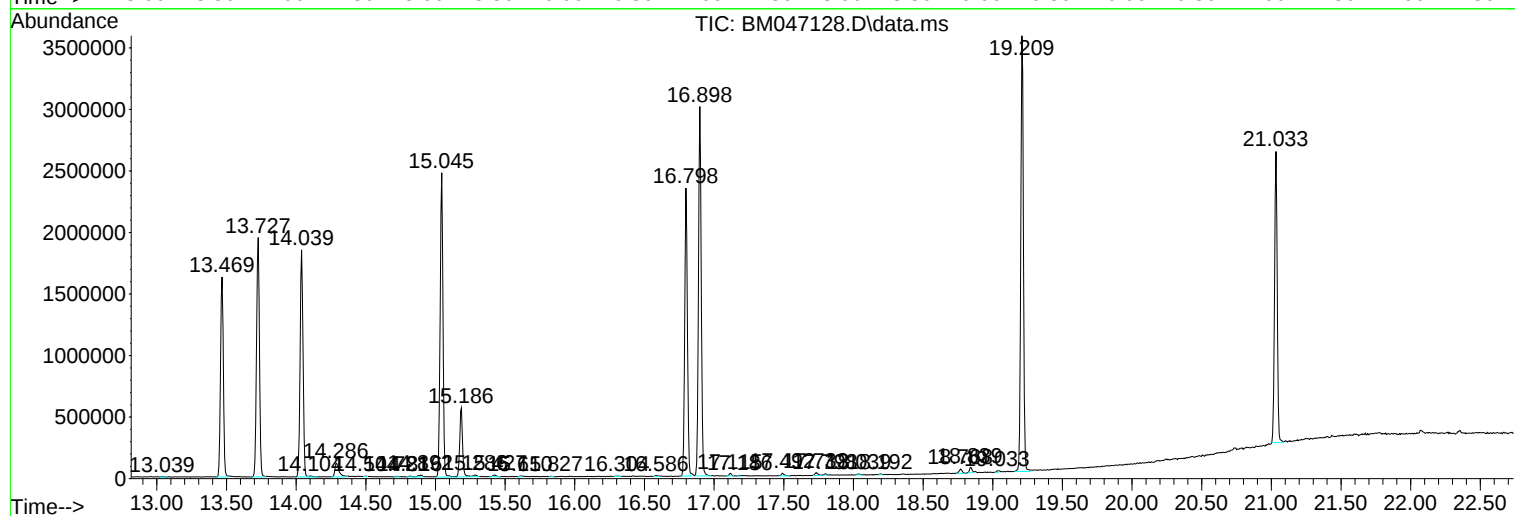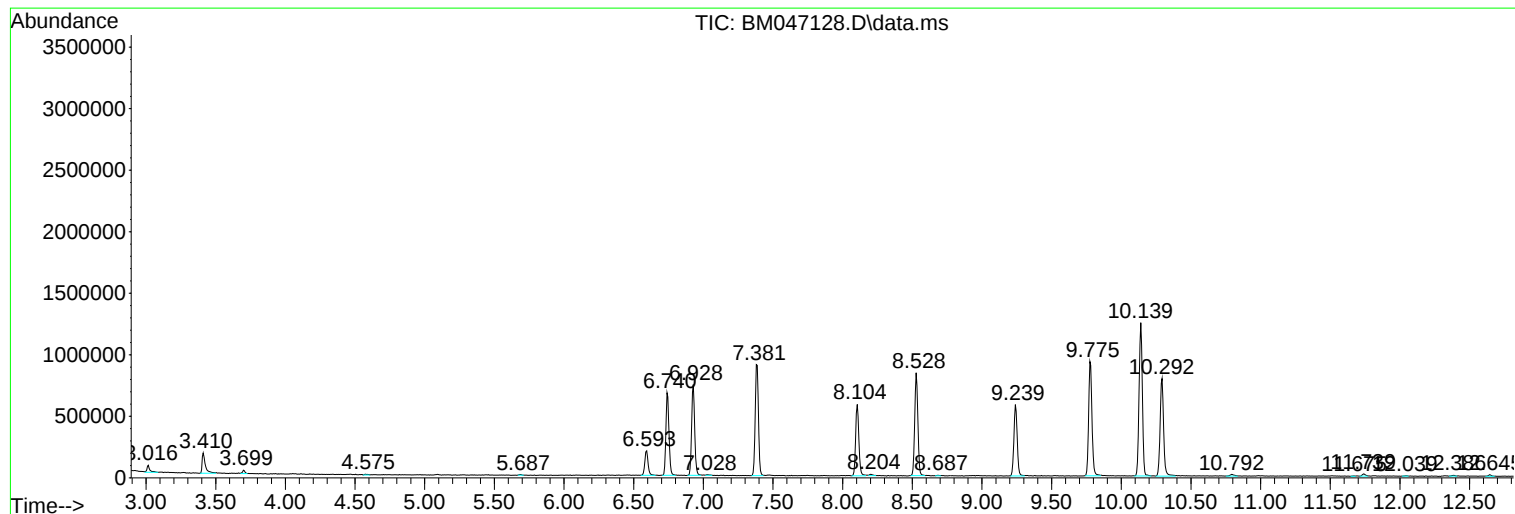

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047128.D
Acq On : 09 Aug 2024 19:44
Operator : RC/JU
Sample : P3480-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047128.D
Acq On : 09 Aug 2024 19:44
Operator : RC/JU
Sample : P3480-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc