

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047129.D
 Acq On : 09 Aug 2024 20:25
 Operator : RC/JU
 Sample : P3480-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	18	22	25	rBV	46960	56817	1.23%	0.122%
2	3.263	60	64	65	rBV4	5151	6882	0.15%	0.015%
3	3.410	85	89	101	rBV	148933	233888	5.08%	0.503%
4	3.610	120	123	127	rVB6	4494	4721	0.10%	0.010%
5	3.699	135	138	143	rVB	26895	30957	0.67%	0.067%
6	4.393	252	256	262	rBV7	3747	8085	0.18%	0.017%
7	4.457	262	267	270	rBV7	6307	9827	0.21%	0.021%
8	4.575	284	287	291	rBV5	3767	5945	0.13%	0.013%
9	5.081	370	373	376	rBV5	4930	7162	0.16%	0.015%
10	5.687	472	476	481	rVB8	6405	8921	0.19%	0.019%
11	6.457	600	607	612	rBV10	3327	9732	0.21%	0.021%
12	6.593	623	630	637	rBV	252905	395561	8.59%	0.851%
13	6.740	648	655	666	rBV	685619	1047892	22.76%	2.253%
14	6.928	679	687	700	rBV	791984	1224524	26.60%	2.633%
15	7.028	700	704	707	rVB6	5488	7775	0.17%	0.017%
16	7.381	757	764	774	rBV	837317	1305883	28.37%	2.808%
17	7.463	774	778	783	rVB5	4828	8502	0.18%	0.018%
18	8.104	880	887	898	rBV	674956	1041662	22.63%	2.240%
19	8.210	901	905	911	rVB5	8811	16958	0.37%	0.036%
20	8.528	952	959	979	rVB	822219	1294927	28.13%	2.784%
21	9.240	1072	1080	1093	rBV	657636	1061370	23.06%	2.282%
22	9.328	1093	1095	1101	rVB7	3148	4691	0.10%	0.010%
23	9.775	1164	1171	1186	rBV	980210	1609947	34.97%	3.462%
24	10.139	1226	1233	1247	rVB	1097873	1797670	39.05%	3.865%
25	10.292	1252	1259	1270	rBV	792549	1335463	29.01%	2.872%
26	10.792	1339	1344	1349	rBV5	9971	18005	0.39%	0.039%
27	11.510	1463	1466	1473	rVB7	3407	5599	0.12%	0.012%
28	11.739	1499	1505	1513	rBV3	17186	33178	0.72%	0.071%
29	12.322	1600	1604	1608	rVB7	3836	5921	0.13%	0.013%
30	12.386	1608	1615	1623	rVB7	8152	17572	0.38%	0.038%
31	12.651	1652	1660	1667	rVB6	12097	24168	0.52%	0.052%
32	13.469	1791	1799	1813	rBV	1658631	2240904	48.68%	4.818%
33	13.727	1834	1843	1853	rBV	1832964	2719738	59.08%	5.848%
34	14.039	1888	1896	1903	rBV	1607839	2294831	49.85%	4.934%
35	14.286	1932	1938	1955	rBV	181505	353624	7.68%	0.760%
36	14.498	1971	1974	1982	rVB9	5644	10080	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047129.D
 Acq On : 09 Aug 2024 20:25
 Operator : RC/JU
 Sample : P3480-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	14.822	2023	2029	2033	rBV5	5175	8491	0.18%	0.018%
38	14.898	2033	2042	2047	rVV4	12441	25998	0.56%	0.056%
39	15.045	2060	2067	2083	rVB	2367213	3364518	73.08%	7.234%
40	15.186	2083	2091	2099	rBV	784224	1100728	23.91%	2.367%
41	15.286	2103	2108	2113	rVB4	17531	23102	0.50%	0.050%
42	15.421	2125	2131	2140	rBV3	12184	23049	0.50%	0.050%
43	15.616	2159	2164	2168	rBV7	6612	10565	0.23%	0.023%
44	16.421	2296	2301	2305	rBV6	4117	6947	0.15%	0.015%
45	16.586	2324	2329	2333	rVV4	5041	9567	0.21%	0.021%
46	16.798	2359	2365	2372	rBV	1920767	2632552	57.18%	5.661%
47	16.898	2376	2382	2394	rVB	2913926	3975196	86.35%	8.548%
48	17.115	2415	2419	2424	rVV	17412	22929	0.50%	0.049%
49	17.192	2428	2432	2435	rVV6	5572	6863	0.15%	0.015%
50	17.404	2464	2468	2472	rVB7	3452	6024	0.13%	0.013%
51	17.492	2479	2483	2488	rBV7	12675	17084	0.37%	0.037%
52	17.733	2520	2524	2530	rBV2	49269	70666	1.54%	0.152%
53	17.798	2532	2535	2540	rVB2	9264	13978	0.30%	0.030%
54	18.033	2572	2575	2576	rBV3	4507	5415	0.12%	0.012%
55	18.768	2696	2700	2705	rBV3	34619	48741	1.06%	0.105%
56	18.845	2709	2713	2717	rVV	37734	50964	1.11%	0.110%
57	19.033	2742	2745	2753	rBV3	41861	51475	1.12%	0.111%
58	19.209	2769	2775	2782	rBV	3296132	4435784	96.35%	9.538%
59	21.033	3080	3085	3092	rBV	2030589	2688540	58.40%	5.781%
60	23.550	3505	3513	3529	rVB	2175380	4603594	100.00%	9.899%
61	23.733	3537	3544	3561	rVB	1278347	3044531	66.13%	6.546%




Sum of corrected areas: 46506683

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047129.D
Acq On : 09 Aug 2024 20:25
Operator : RC/JU
Sample : P3480-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

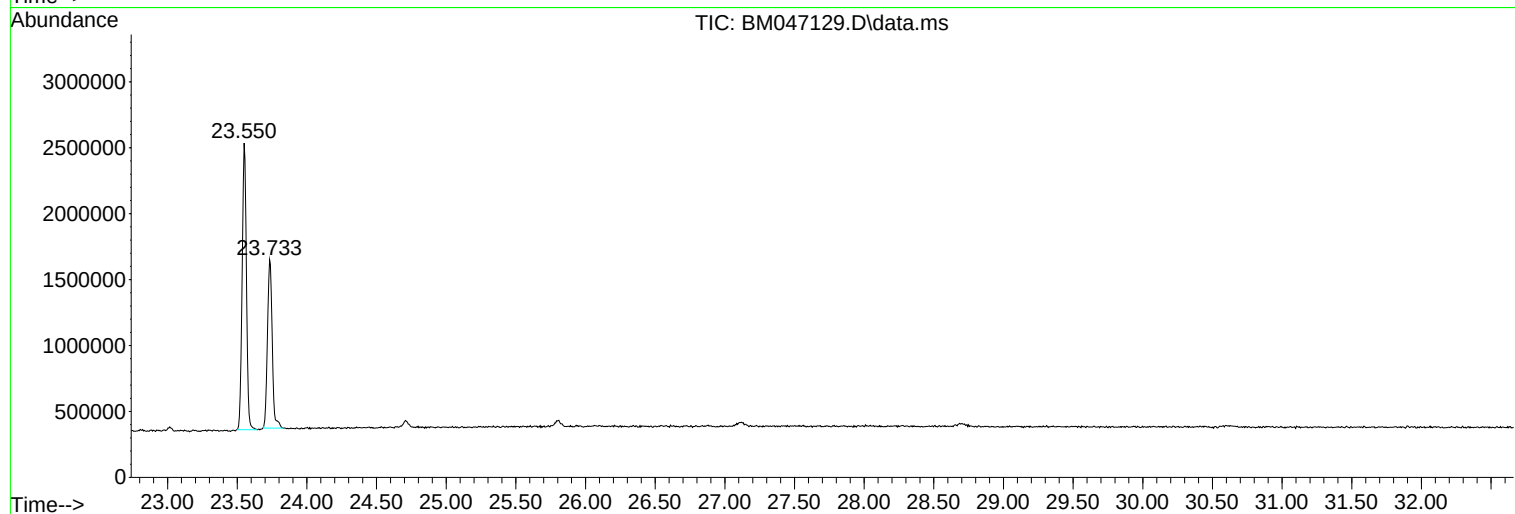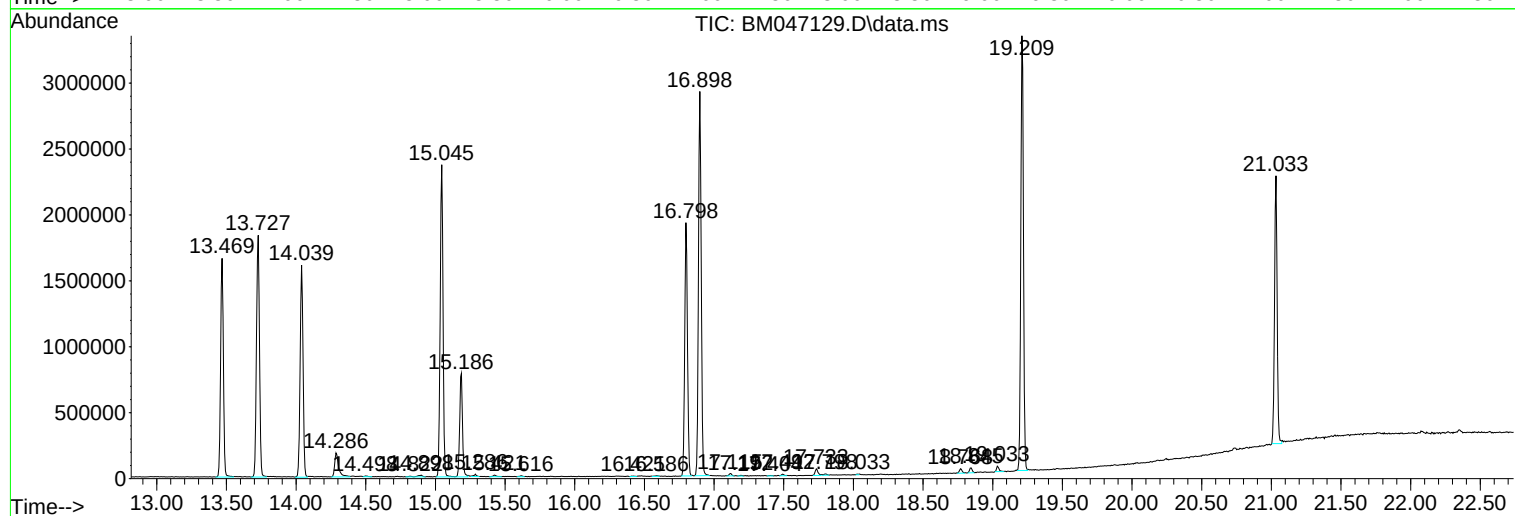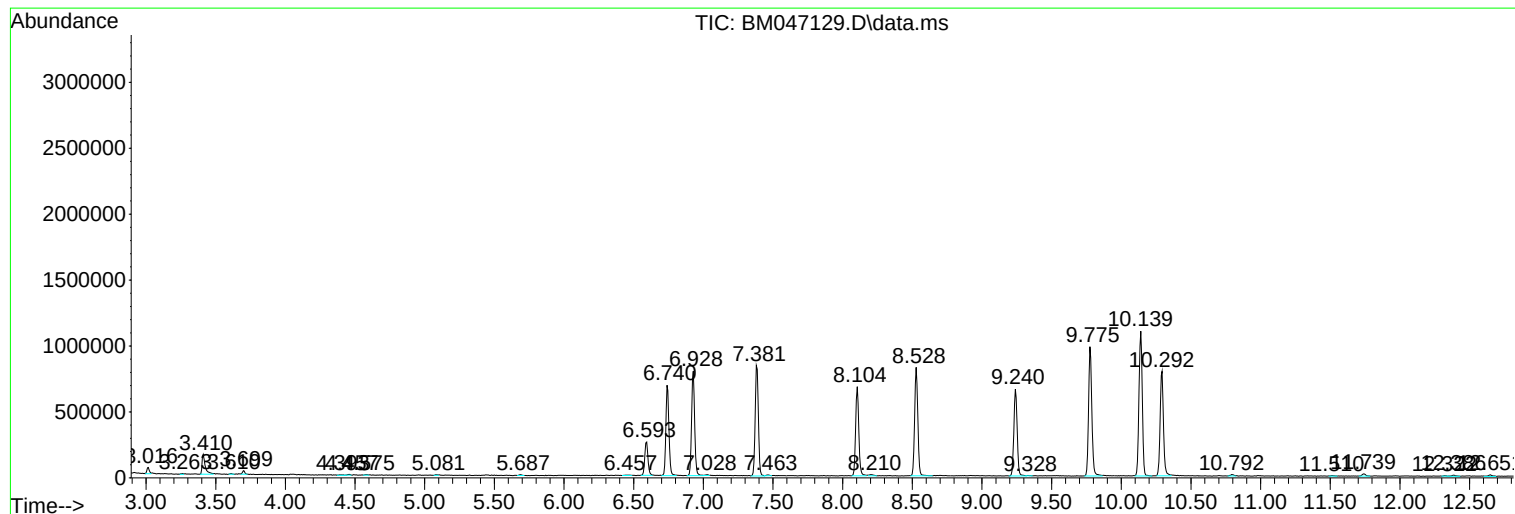

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047129.D
Acq On : 09 Aug 2024 20:25
Operator : RC/JU
Sample : P3480-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047129.D
Acq On : 09 Aug 2024 20:25
Operator : RC/JU
Sample : P3480-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc