

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047132.D
 Acq On : 09 Aug 2024 22:27
 Operator : RC/JU
 Sample : P3529-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	18	22	33	rVB	51473	80282	1.62%	0.155%
2	3.410	86	89	99	rBV	149652	221823	4.48%	0.427%
3	3.669	129	133	135	rBV5	6885	8022	0.16%	0.015%
4	3.704	135	139	142	rVB	19203	24164	0.49%	0.047%
5	4.398	254	257	260	rBV5	4525	5529	0.11%	0.011%
6	4.451	265	266	272	rVB5	5582	7281	0.15%	0.014%
7	4.546	279	282	285	rBV4	4207	6586	0.13%	0.013%
8	4.581	285	288	291	rVB5	4419	5143	0.10%	0.010%
9	5.157	382	386	389	rBV4	4306	5759	0.12%	0.011%
10	5.681	472	475	481	rVB8	5554	8886	0.18%	0.017%
11	6.592	624	630	642	rVB	246857	392199	7.92%	0.755%
12	6.740	649	655	665	rBV	879539	1312256	26.50%	2.526%
13	6.928	678	687	698	rBV	944382	1469880	29.68%	2.830%
14	7.028	701	704	711	rVB7	8161	11706	0.24%	0.023%
15	7.381	756	764	772	rBV	890473	1388122	28.03%	2.672%
16	8.104	880	887	898	rBV	712397	1136061	22.94%	2.187%
17	8.528	952	959	968	rBV	1029464	1613777	32.59%	3.107%
18	8.969	1029	1034	1038	rBV2	15138	22712	0.46%	0.044%
19	9.239	1073	1080	1095	rBV	844088	1336552	26.99%	2.573%
20	9.522	1123	1128	1130	rBV3	4881	6364	0.13%	0.012%
21	9.775	1163	1171	1185	rBV	1219811	2002735	40.44%	3.856%
22	10.139	1225	1233	1242	rBV	1196652	1922204	38.81%	3.700%
23	10.292	1250	1259	1268	rBV	791098	1380197	27.87%	2.657%
24	10.904	1360	1363	1368	rBV5	5781	12088	0.24%	0.023%
25	10.980	1372	1376	1383	rVB9	5839	14277	0.29%	0.027%
26	11.457	1452	1457	1462	rVB	18996	29856	0.60%	0.057%
27	11.739	1499	1505	1514	rBV	24050	46048	0.93%	0.089%
28	12.392	1610	1616	1621	rVB9	3904	7879	0.16%	0.015%
29	12.657	1656	1661	1666	rVB5	5235	10560	0.21%	0.020%
30	12.957	1706	1712	1716	rBV9	3359	5942	0.12%	0.011%
31	13.468	1792	1799	1809	rBV	2009174	2660161	53.72%	5.121%
32	13.727	1836	1843	1854	rBV	2249959	3337401	67.39%	6.425%
33	14.039	1889	1896	1907	rBV	1702746	2460097	49.68%	4.736%
34	14.286	1933	1938	1953	rBV	146114	295197	5.96%	0.568%
35	14.410	1957	1959	1963	rVV5	4275	5552	0.11%	0.011%
36	14.498	1971	1974	1978	rVB5	4805	7545	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
 Data File : BM047132.D
 Acq On : 09 Aug 2024 22:27
 Operator : RC/JU
 Sample : P3529-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	14.886	2036	2040	2042	rBV4	4613	5563	0.11%	0.011%
38	15.045	2060	2067	2075	rBV	2814471	4003540	80.84%	7.707%
39	15.180	2084	2090	2104	rBV	842558	1213129	24.50%	2.335%
40	15.286	2104	2108	2115	rVB5	17705	28657	0.58%	0.055%
41	15.615	2159	2164	2170	rBV8	6219	13336	0.27%	0.026%
42	16.592	2325	2330	2335	rVB7	8286	13841	0.28%	0.027%
43	16.798	2358	2365	2372	rBV	2135668	2875892	58.07%	5.536%
44	16.898	2376	2382	2395	rVV	3215660	4397703	88.80%	8.466%
45	17.115	2417	2419	2425	rVV5	5802	8494	0.17%	0.016%
46	17.198	2431	2433	2436	rVB4	5623	5777	0.12%	0.011%
47	17.409	2465	2469	2473	rBV7	4117	7719	0.16%	0.015%
48	17.733	2518	2524	2532	rBV6	30426	54297	1.10%	0.105%
49	17.798	2532	2535	2539	rVV3	7642	9970	0.20%	0.019%
50	18.203	2600	2604	2609	rBV6	3718	6437	0.13%	0.012%
51	18.768	2696	2700	2706	rVB2	39008	51863	1.05%	0.100%
52	18.845	2708	2713	2718	rBV	45202	67936	1.37%	0.131%
53	19.033	2742	2745	2749	rBV5	14053	21747	0.44%	0.042%
54	19.209	2769	2775	2782	rBV	3669682	4889067	98.72%	9.412%
55	21.033	3080	3085	3091	rBV	2157027	2847350	57.50%	5.482%
56	23.550	3505	3513	3522	rBV	2283587	4952275	100.00%	9.534%
57	23.733	3537	3544	3559	rVB	1435198	3209127	64.80%	6.178%




Sum of corrected areas: 51944563

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047132.D
Acq On : 09 Aug 2024 22:27
Operator : RC/JU
Sample : P3529-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

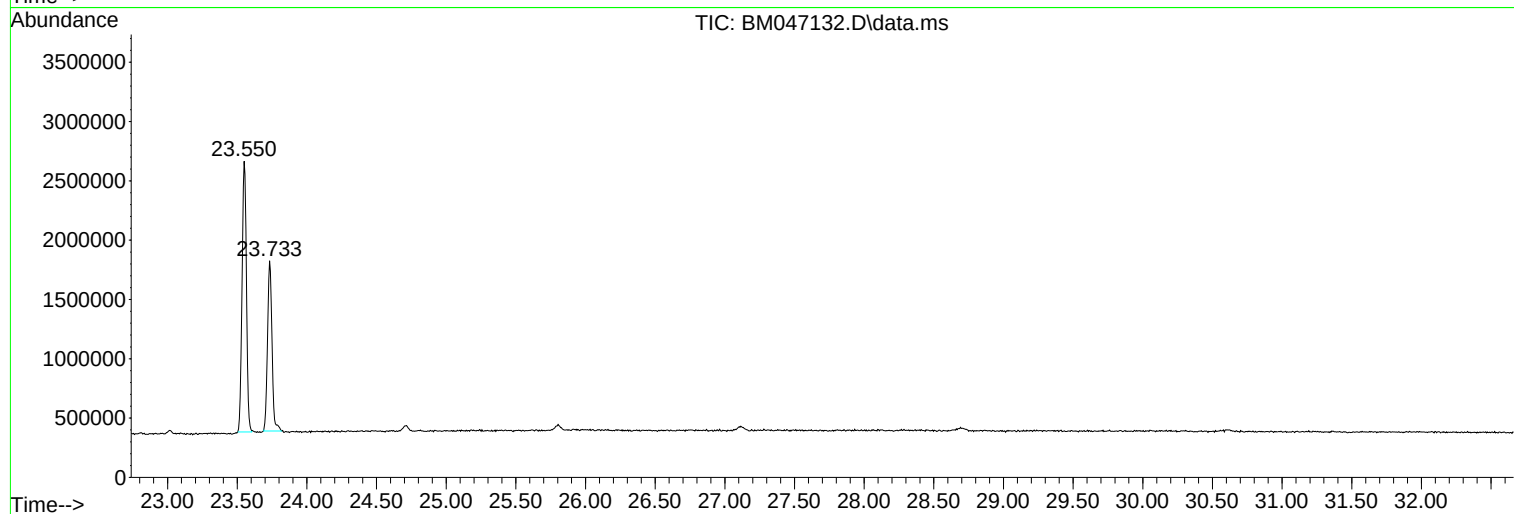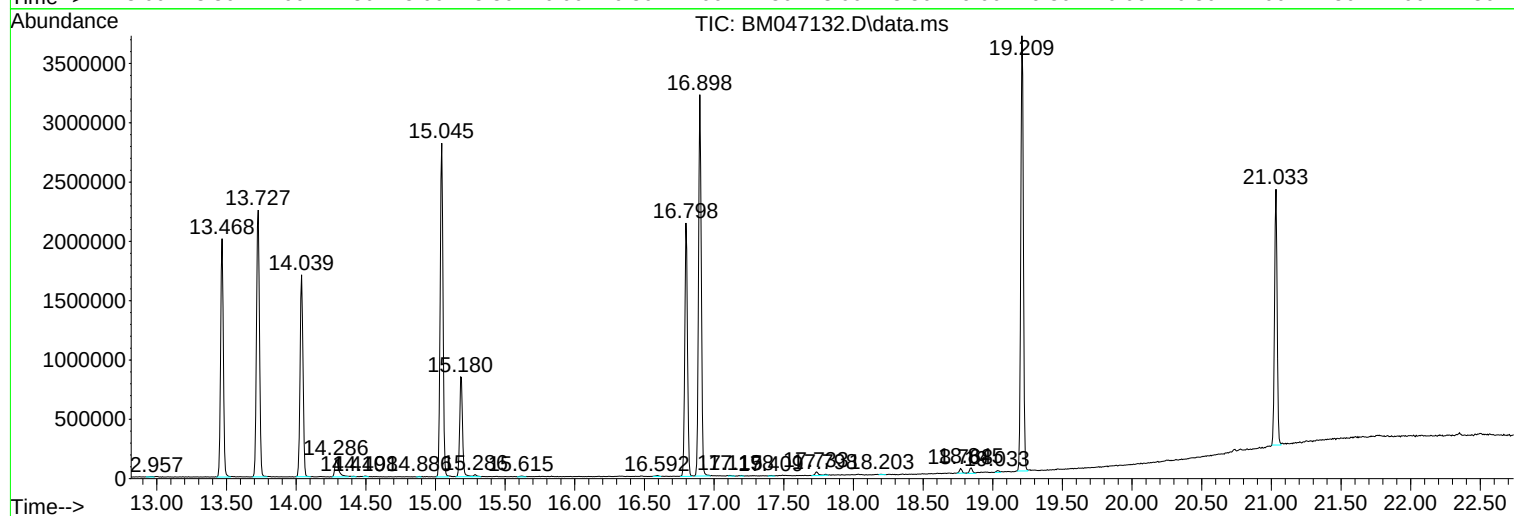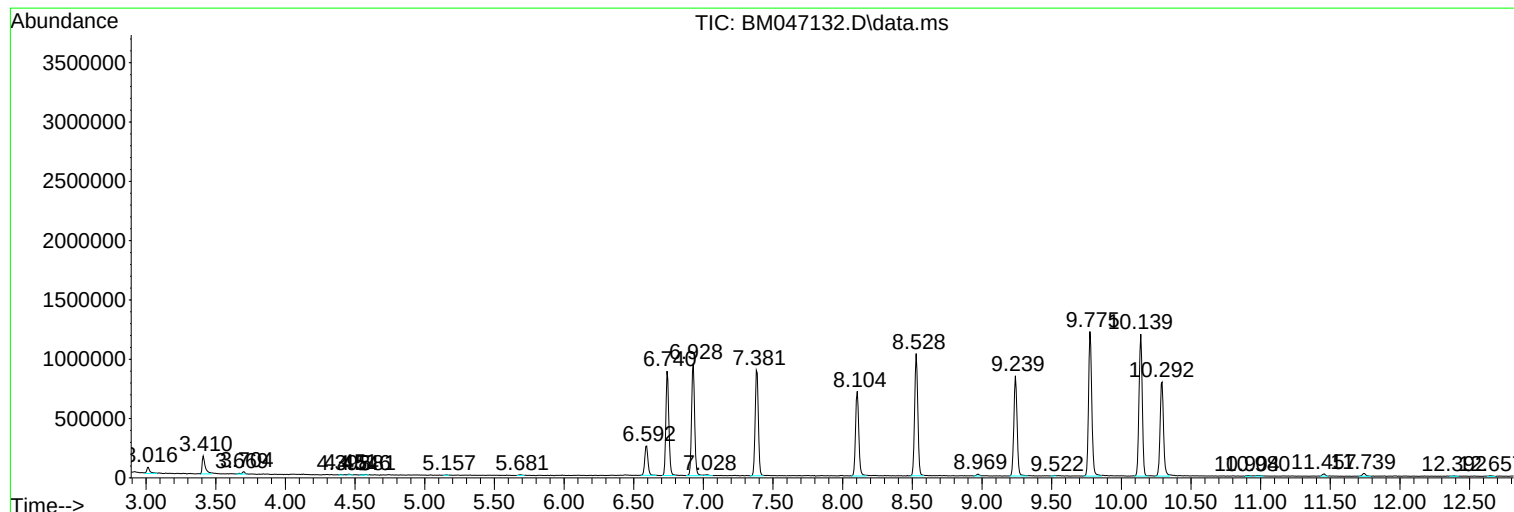

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047132.D
Acq On : 09 Aug 2024 22:27
Operator : RC/JU
Sample : P3529-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080924\
Data File : BM047132.D
Acq On : 09 Aug 2024 22:27
Operator : RC/JU
Sample : P3529-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc