


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082119\
 Data File : BM022219.D
 Acq On : 21 Aug 2019 08:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 02:18:05 2019

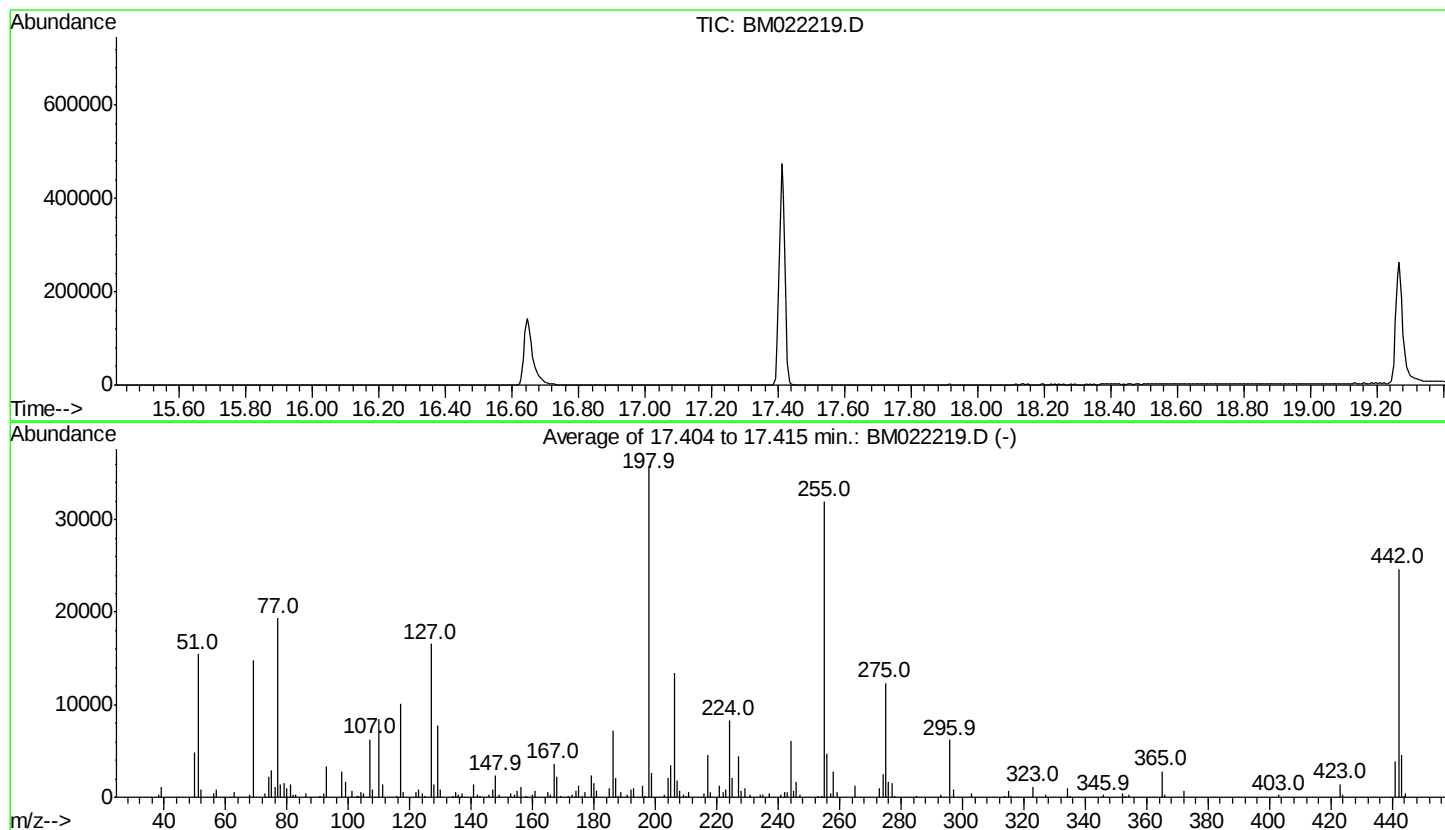

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	15467	PASS
68	69	0.00	2	1.7	256	PASS
69	198	0.00	100	41.5	14861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.3	16598	PASS
197	198	0.00	2	0.3	118	PASS
198	198	100	100	100.0	35845	PASS
199	198	5	9	7.3	2615	PASS
275	198	10	60	34.5	12380	PASS
365	198	1	100	7.8	2809	PASS
441	198	0.01	100	10.9	3906	PASS
442	198	50	100	68.8	24664	PASS
443	442	15	24	18.5	4560	PASS