

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003884.D
 Acq On : 30 Dec 2015 17:42
 Operator : SJ/UM
 Sample : G4868-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.875	131	134	138	rBV	2292	3029	0.29%	0.031%
2	4.399	220	223	226	rBB	6292	7136	0.69%	0.072%
3	5.340	380	383	387	rBB	2827	3377	0.33%	0.034%
4	5.687	439	442	445	rBB	1380	1640	0.16%	0.017%
5	6.852	635	640	647	rVB	44707	66093	6.39%	0.668%
6	7.010	661	667	678	rBB	139144	218180	21.09%	2.205%
7	7.204	694	700	709	rBB	156443	240158	23.22%	2.427%
8	7.669	774	779	787	rBB	151041	235946	22.81%	2.385%
9	8.387	895	901	910	rBB	137488	215482	20.83%	2.178%
10	8.828	970	976	986	rBB	170041	269193	26.02%	2.721%
11	9.545	1093	1098	1106	rBB	140008	225883	21.84%	2.283%
12	10.087	1184	1190	1201	rBB	227272	371772	35.94%	3.758%
13	10.457	1246	1253	1262	rBB	220056	364204	35.21%	3.681%
14	10.610	1274	1279	1284	rBB	4166	6012	0.58%	0.061%
15	12.057	1522	1525	1529	rBB	2390	3377	0.33%	0.034%
16	13.739	1805	1811	1821	rBB	437000	606114	58.59%	6.126%
17	14.016	1852	1858	1874	rBV	506623	725923	70.17%	7.337%
18	14.169	1879	1884	1893	rBV	4367	8845	0.86%	0.089%
19	14.328	1905	1911	1918	rBB2	314453	463817	44.84%	4.688%
20	14.551	1944	1949	1960	rBB	26144	44186	4.27%	0.447%
21	14.751	1978	1983	1988	rBB	12404	14936	1.44%	0.151%
22	15.322	2074	2080	2089	rBB	650611	916674	88.61%	9.265%
23	15.451	2097	2102	2109	rBB	172325	223638	21.62%	2.260%
24	15.563	2118	2121	2124	rBB	4765	4930	0.48%	0.050%
25	17.074	2372	2378	2385	rBV2	360786	499186	48.25%	5.045%
26	17.174	2389	2395	2410	rVV2	673335	941014	90.96%	9.511%
27	19.110	2721	2724	2730	rVB	5666	7260	0.70%	0.073%
28	19.251	2747	2748	2753	rBV	1035	1125	0.11%	0.011%
29	19.368	2763	2768	2771	rBV	4103	5196	0.50%	0.053%
30	19.480	2781	2787	2795	rBV	774776	1034487	100.00%	10.456%
31	20.409	2942	2945	2949	rVB2	2099	2329	0.23%	0.024%
32	20.633	2979	2983	2986	rBV	2155	3044	0.29%	0.031%
33	20.945	3034	3036	3039	rBV2	1058	1400	0.14%	0.014%
34	20.992	3041	3044	3048	rVV3	1360	2028	0.20%	0.020%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003884.D
Acq On : 30 Dec 2015 17:42
Operator : SJ/UM
Sample : G4868-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION

35	21.056	3051	3055	3059	rVV	4065	5465	0.53%	0.055%
36	21.280	3087	3093	3099	rBV	416439	527960	51.04%	5.336%
37	21.351	3104	3105	3107	rBV2	1527	1413	0.14%	0.014%
38	21.427	3115	3118	3121	rVB2	3059	2581	0.25%	0.026%
39	21.633	3151	3153	3156	rBV4	1787	2387	0.23%	0.024%
40	21.856	3188	3191	3194	rVB2	4146	4727	0.46%	0.048%
41	22.315	3266	3269	3277	rVB3	9198	12640	1.22%	0.128%
42	22.780	3345	3348	3351	rBV2	4339	5996	0.58%	0.061%
43	22.821	3351	3355	3362	rVB2	11013	16250	1.57%	0.164%
44	23.374	3441	3449	3461	rBV	540968	996500	96.33%	10.072%
45	23.515	3466	3473	3488	rVB	269519	504243	48.74%	5.096%
46	24.021	3554	3559	3566	rVB2	13767	25503	2.47%	0.258%
47	24.756	3679	3684	3691	rVB2	13612	29379	2.84%	0.297%
48	25.621	3827	3831	3839	rVB4	9217	21311	2.06%	0.215%


Sum of corrected areas: 9893969

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003884.D
Acq On : 30 Dec 2015 17:42
Operator : SJ/UM
Sample : G4868-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

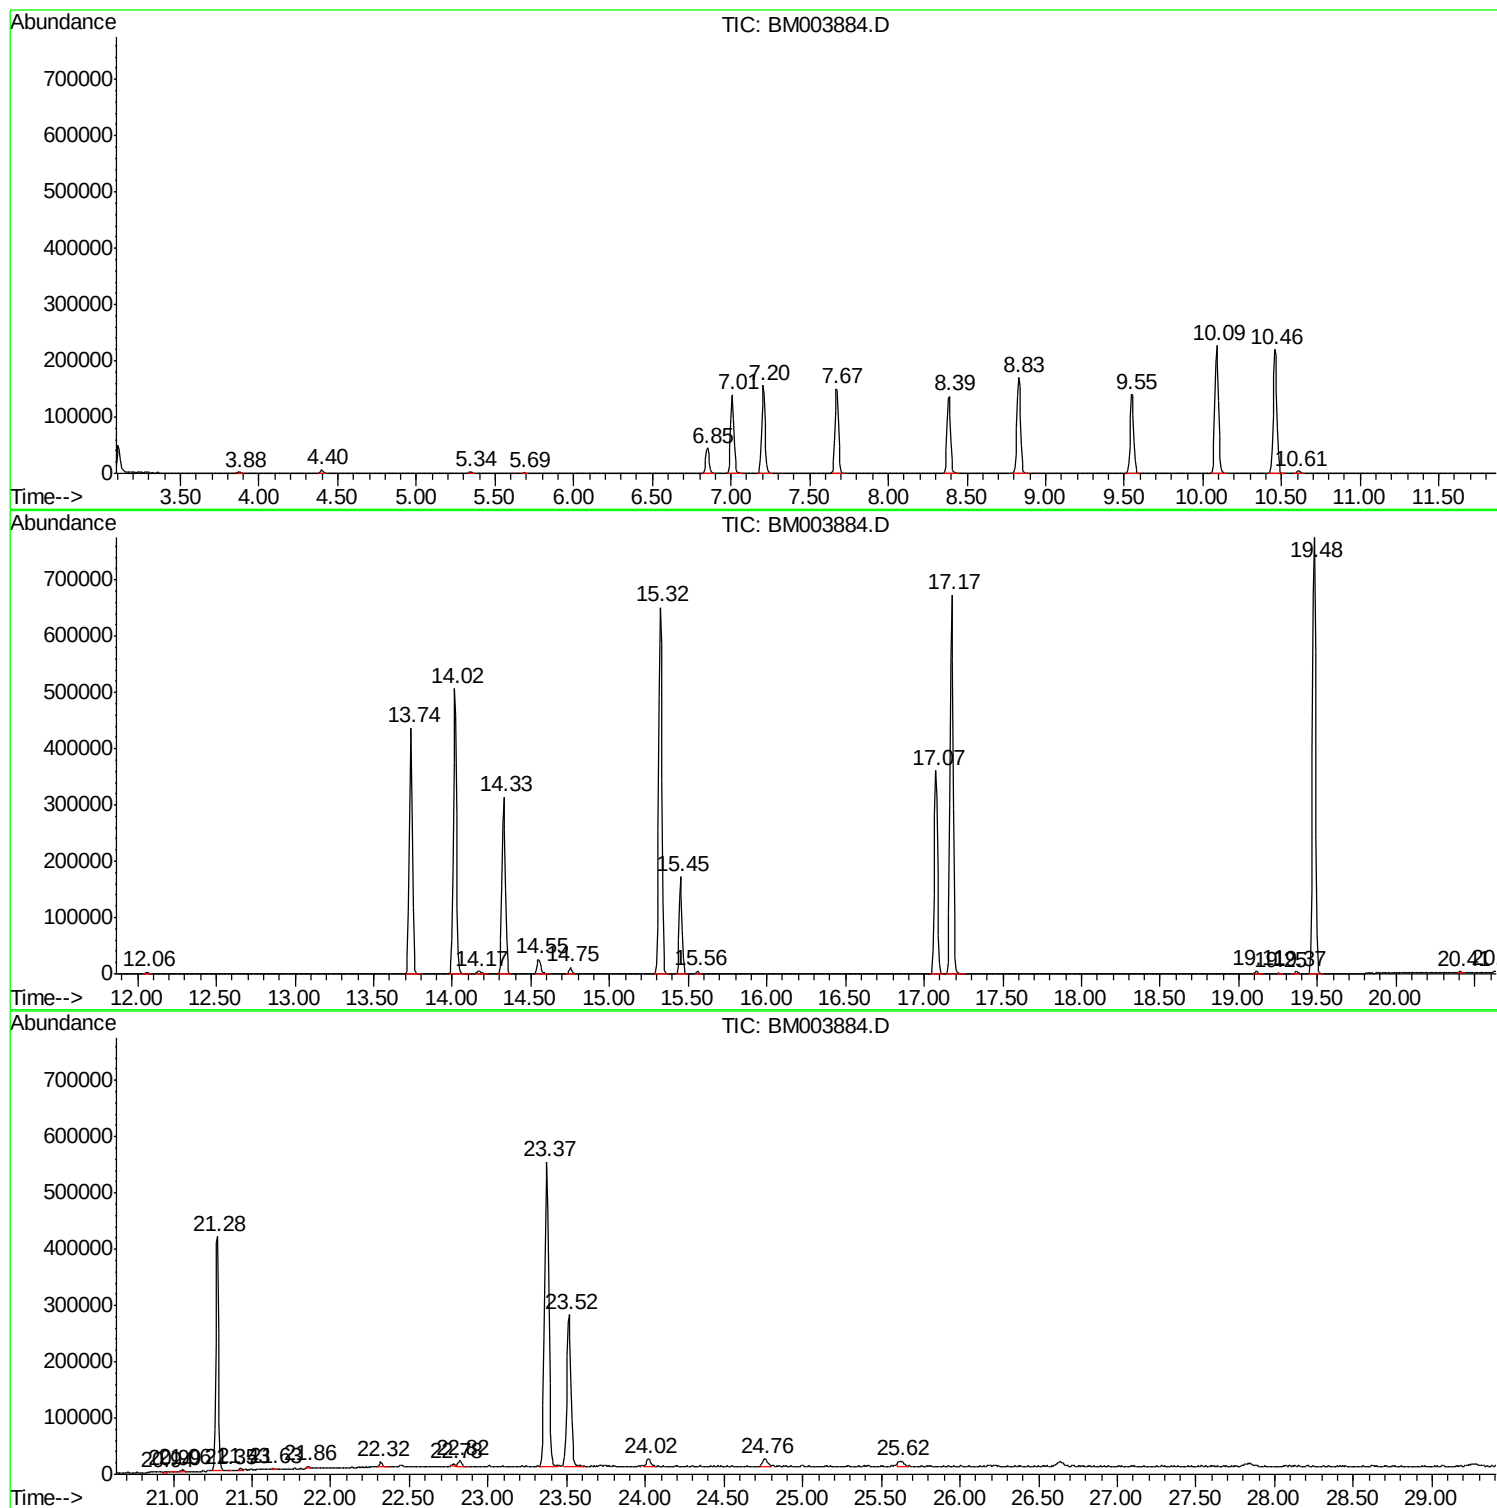

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003884.D
Acq On : 30 Dec 2015 17:42
Operator : SJ/UM
Sample : G4868-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003884.D
Acq On : 30 Dec 2015 17:42
Operator : SJ/UM
Sample : G4868-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc