

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003885.D
 Acq On : 30 Dec 2015 18:17
 Operator : SJ/UM
 Sample : G4868-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43M7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.875	129	134	137	rBV2	2042	2808	0.27%	0.027%
2	4.399	220	223	226	rBB	5757	7160	0.69%	0.069%
3	4.999	321	325	328	rBB	2680	3204	0.31%	0.031%
4	5.340	380	383	387	rBB	2838	3470	0.34%	0.033%
5	5.687	439	442	445	rBB	1368	1632	0.16%	0.016%
6	6.851	634	640	647	rBB	44741	64322	6.24%	0.618%
7	7.004	661	666	673	rBV	141040	217935	21.13%	2.093%
8	7.204	694	700	709	rBB	155960	238827	23.16%	2.293%
9	7.669	773	779	788	rBB	177869	278619	27.02%	2.676%
10	8.387	895	901	910	rBB	134975	210309	20.39%	2.020%
11	8.828	970	976	986	rBB	171617	270106	26.19%	2.594%
12	9.551	1093	1099	1106	rBB	140020	228270	22.13%	2.192%
13	10.087	1184	1190	1202	rBB	227909	366766	35.56%	3.522%
14	10.457	1246	1253	1263	rBB	258212	427901	41.49%	4.109%
15	10.610	1275	1279	1283	rBB	1486	2024	0.20%	0.019%
16	12.057	1522	1525	1529	rBB	2380	3376	0.33%	0.032%
17	13.739	1805	1811	1820	rVB	442841	616606	59.79%	5.921%
18	14.016	1852	1858	1865	rBV	502114	724902	70.29%	6.961%
19	14.169	1879	1884	1891	rBV	5173	10197	0.99%	0.098%
20	14.327	1905	1911	1918	rBB2	371758	551852	53.51%	5.299%
21	14.551	1944	1949	1957	rBV	26770	42808	4.15%	0.411%
22	14.751	1978	1983	1986	rBB	3821	4657	0.45%	0.045%
23	15.321	2074	2080	2089	rBB	654786	925732	89.76%	8.890%
24	15.451	2097	2102	2109	rBB	182185	227943	22.10%	2.189%
25	15.563	2118	2121	2124	rBB	4373	4904	0.48%	0.047%
26	16.863	2339	2342	2345	rBB	1038	1213	0.12%	0.012%
27	17.074	2372	2378	2385	rBV2	426936	597523	57.94%	5.738%
28	17.174	2389	2395	2410	rVV2	695526	955751	92.67%	9.178%
29	19.109	2721	2724	2730	rBV	5111	6164	0.60%	0.059%
30	19.368	2763	2768	2772	rVB	4401	5323	0.52%	0.051%
31	19.480	2781	2787	2795	rBV	744419	1031341	100.00%	9.904%
32	20.080	2887	2889	2893	rBV3	1061	1265	0.12%	0.012%
33	20.409	2941	2945	2947	rBV3	1583	1400	0.14%	0.013%
34	20.633	2979	2983	2986	rVV	3689	3853	0.37%	0.037%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003885.D
Acq On : 30 Dec 2015 18:17
Operator : SJ/UM
Sample : G4868-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION

35	21.056	3051	3055	3059	rBV	5432	6980	0.68%	0.067%
36	21.245	3085	3087	3088	rBV2	1602	1341	0.13%	0.013%
37	21.280	3088	3093	3100	rVB	481248	616195	59.75%	5.917%
38	21.427	3115	3118	3121	rBV2	2639	2981	0.29%	0.029%
39	21.856	3188	3191	3197	rVB3	4407	6849	0.66%	0.066%
40	22.315	3266	3269	3274	rVB	10126	12658	1.23%	0.122%
41	22.780	3345	3348	3351	rBV3	4700	6153	0.60%	0.059%
42	22.821	3351	3355	3360	rVB	12654	17903	1.74%	0.172%
43	22.992	3382	3384	3391	rVB4	5518	9757	0.95%	0.094%
44	23.374	3441	3449	3459	rBV	537355	984989	95.51%	9.459%
45	23.515	3465	3473	3486	rVB	314507	584935	56.72%	5.617%
46	23.703	3501	3505	3511	rBV6	6527	11732	1.14%	0.113%
47	24.021	3553	3559	3566	rBV2	15998	31748	3.08%	0.305%
48	24.762	3679	3685	3695	rVB	16361	36120	3.50%	0.347%
49	25.621	3826	3831	3838	rVB3	10944	25296	2.45%	0.243%
50	26.644	3999	4005	4010	rVB3	7310	17528	1.70%	0.168%


Sum of corrected areas: 10413328

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003885.D
Acq On : 30 Dec 2015 18:17
Operator : SJ/UM
Sample : G4868-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

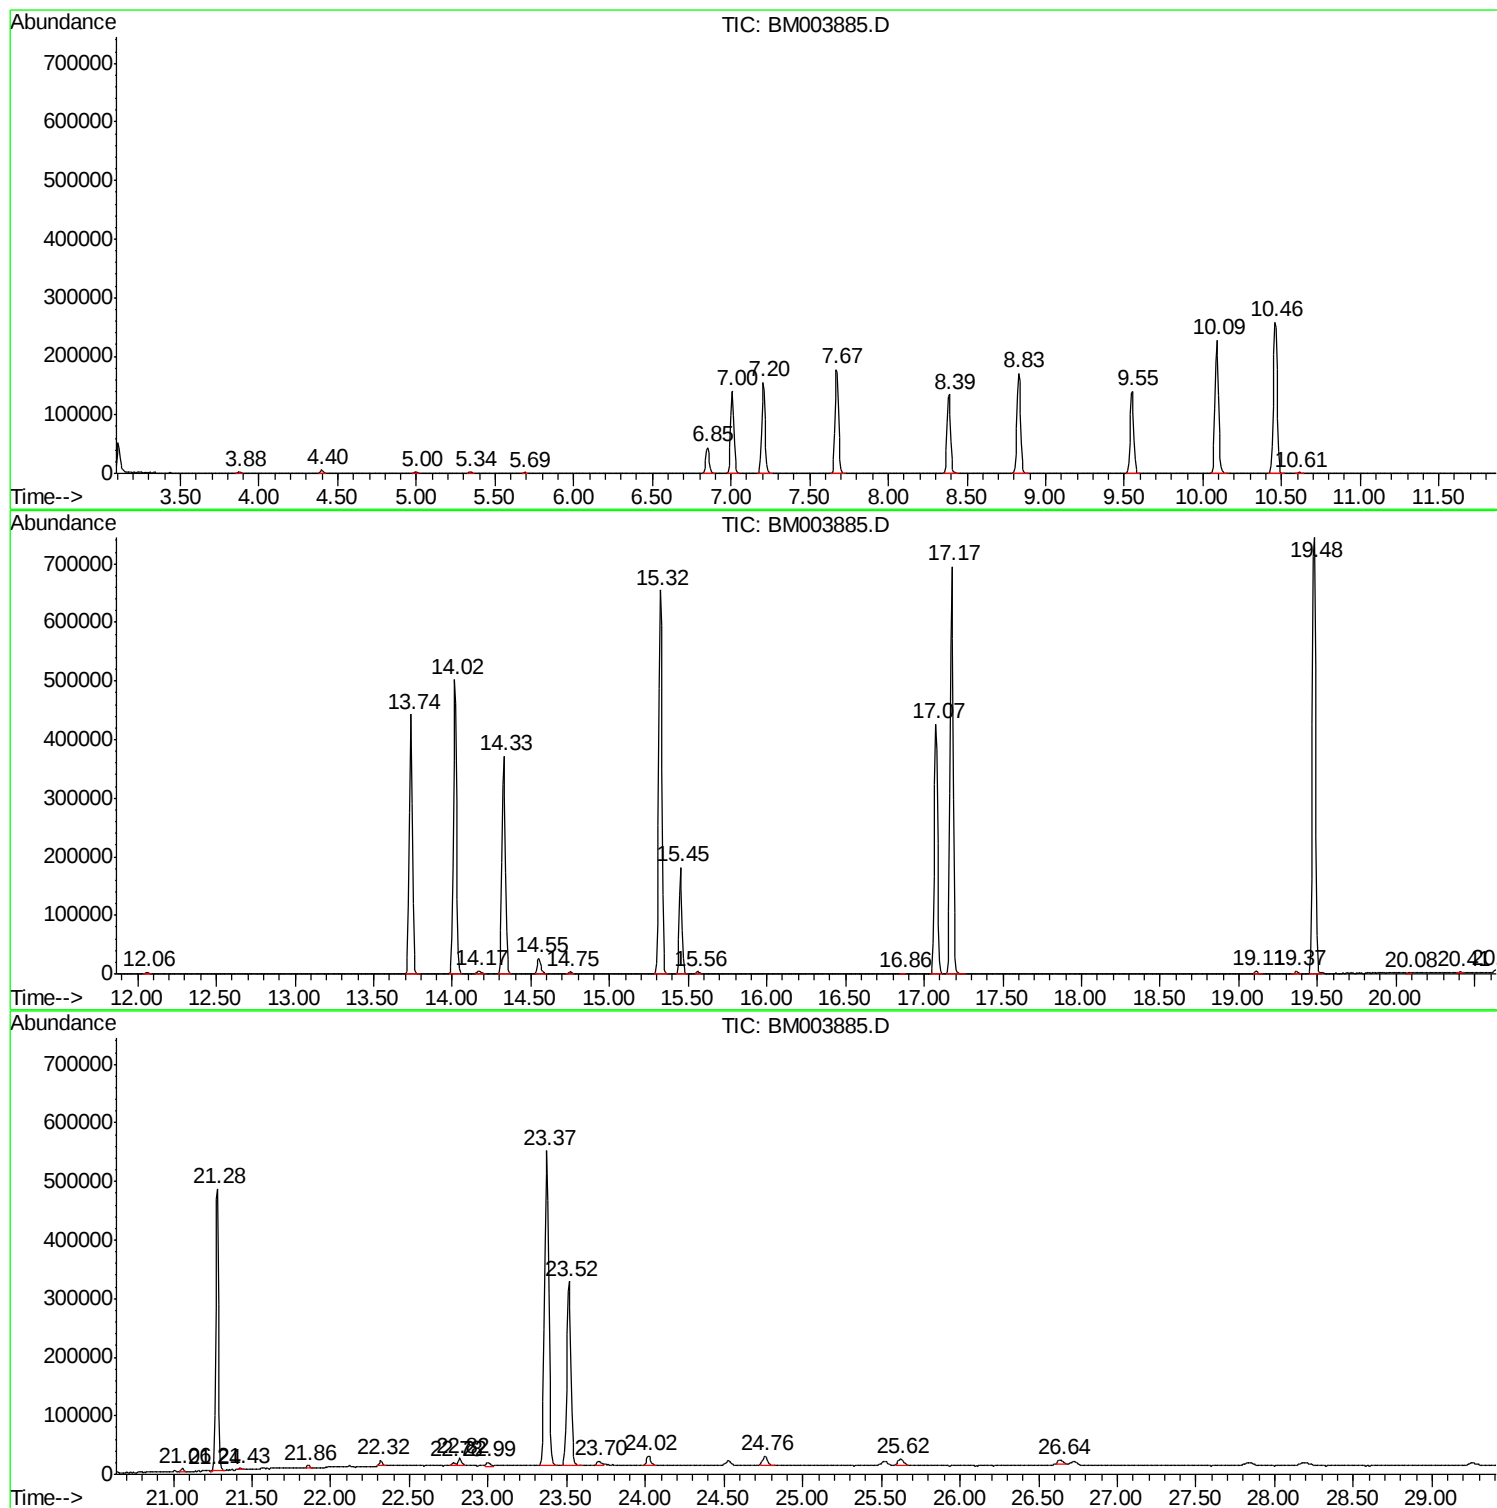

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003885.D
Acq On : 30 Dec 2015 18:17
Operator : SJ/UM
Sample : G4868-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003885.D
Acq On : 30 Dec 2015 18:17
Operator : SJ/UM
Sample : G4868-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc