

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003886.D
 Acq On : 30 Dec 2015 18:53
 Operator : SJ/UM
 Sample : G4868-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43M8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	12	rVB	1864	1909	0.23%	0.021%
2	4.316	206	209	212	rBV	484	903	0.11%	0.010%
3	4.998	321	325	328	rBB	3004	3343	0.41%	0.038%
4	6.851	635	640	647	rBB	39713	57877	7.09%	0.651%
5	7.004	661	666	676	rBB	106560	165963	20.32%	1.867%
6	7.204	695	700	708	rBB	122667	185388	22.69%	2.086%
7	7.669	773	779	787	rBB	182336	284771	34.86%	3.204%
8	8.386	895	901	910	rBB	113817	174908	21.41%	1.968%
9	8.828	970	976	985	rBB	129754	203977	24.97%	2.295%
10	9.551	1093	1099	1105	rBV	107452	169765	20.78%	1.910%
11	10.086	1184	1190	1201	rBB	176367	282237	34.55%	3.176%
12	10.457	1247	1253	1260	rBV	264163	442041	54.11%	4.974%
13	12.057	1522	1525	1529	rBB2	1789	2236	0.27%	0.025%
14	12.351	1572	1575	1579	rBB	1911	2578	0.32%	0.029%
15	13.739	1805	1811	1816	rBV	353860	490813	60.08%	5.523%
16	13.780	1816	1818	1823	rVB	8377	9577	1.17%	0.108%
17	14.016	1852	1858	1868	rBV	382008	536091	65.63%	6.032%
18	14.168	1878	1884	1890	rBV	6059	10692	1.31%	0.120%
19	14.227	1890	1894	1897	rVB	3299	4224	0.52%	0.048%
20	14.327	1905	1911	1918	rBB2	394392	586220	71.76%	6.596%
21	14.386	1919	1921	1924	rBB	1226	1175	0.14%	0.013%
22	14.551	1944	1949	1959	rBB	24139	39961	4.89%	0.450%
23	15.180	2053	2056	2059	rBB	4270	4888	0.60%	0.055%
24	15.321	2074	2080	2087	rBV	505379	708053	86.68%	7.967%
25	15.380	2087	2090	2092	rVB	1395	1562	0.19%	0.018%
26	15.451	2097	2102	2108	rBV	135772	171569	21.00%	1.931%
27	15.562	2118	2121	2127	rBB2	3282	4375	0.54%	0.049%
28	16.039	2199	2202	2209	rBB	4753	7233	0.89%	0.081%
29	16.833	2334	2337	2340	rBV	3420	3960	0.48%	0.045%
30	16.862	2340	2342	2345	rVB	1116	1176	0.14%	0.013%
31	17.074	2372	2378	2384	rBV2	463880	642288	78.63%	7.227%
32	17.115	2384	2385	2389	rVV	2765	2482	0.30%	0.028%
33	17.174	2389	2395	2411	rVB	544515	762950	93.40%	8.585%
34	17.568	2460	2462	2465	rBB	1387	1262	0.15%	0.014%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003886.D
Acq On : 30 Dec 2015 18:53
Operator : SJ/UM
Sample : G4868-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION

35	17.968	2527	2530	2533	rBB	3267	3381	0.41%	0.038%
36	18.045	2540	2543	2546	rBB	1002	1198	0.15%	0.013%
37	19.109	2721	2724	2729	rBB	3665	4250	0.52%	0.048%
38	19.256	2746	2749	2753	rBV	2665	3198	0.39%	0.036%
39	19.362	2763	2767	2771	rBV	3472	3828	0.47%	0.043%
40	19.480	2781	2787	2795	rBV	598738	816892	100.00%	9.192%
41	19.733	2827	2830	2833	rVB2	712	1012	0.12%	0.011%
42	20.327	2928	2931	2932	rBV	818	863	0.11%	0.010%
43	20.456	2945	2953	2958	rBV5	1596	4802	0.59%	0.054%
44	20.556	2967	2970	2974	rBV4	767	938	0.11%	0.011%
45	20.633	2980	2983	2986	rBV	1277	1760	0.22%	0.020%
46	20.850	3018	3020	3023	rBV4	576	869	0.11%	0.010%
47	20.944	3034	3036	3038	rBV2	999	1098	0.13%	0.012%
48	20.986	3040	3043	3048	rVB3	3168	4848	0.59%	0.055%
49	21.056	3051	3055	3059	rBV	4832	6482	0.79%	0.073%
50	21.244	3085	3087	3088	rVV2	1125	1016	0.12%	0.011%
51	21.280	3088	3093	3101	rVV	510539	643189	78.74%	7.237%
52	21.862	3188	3192	3194	rBV4	3826	5139	0.63%	0.058%
53	22.321	3266	3270	3274	rBV2	6384	8662	1.06%	0.097%
54	22.821	3351	3355	3359	rVB	8131	9941	1.22%	0.112%
55	23.374	3441	3449	3458	rBV	411868	751421	91.99%	8.455%
56	23.515	3466	3473	3484	rVB	330228	604690	74.02%	6.804%
57	24.021	3554	3559	3566	rBV2	10706	20407	2.50%	0.230%
58	24.762	3682	3685	3692	rVB2	10361	18699	2.29%	0.210%


Sum of corrected areas: 8887030

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003886.D
Acq On : 30 Dec 2015 18:53
Operator : SJ/UM
Sample : G4868-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
E43M8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

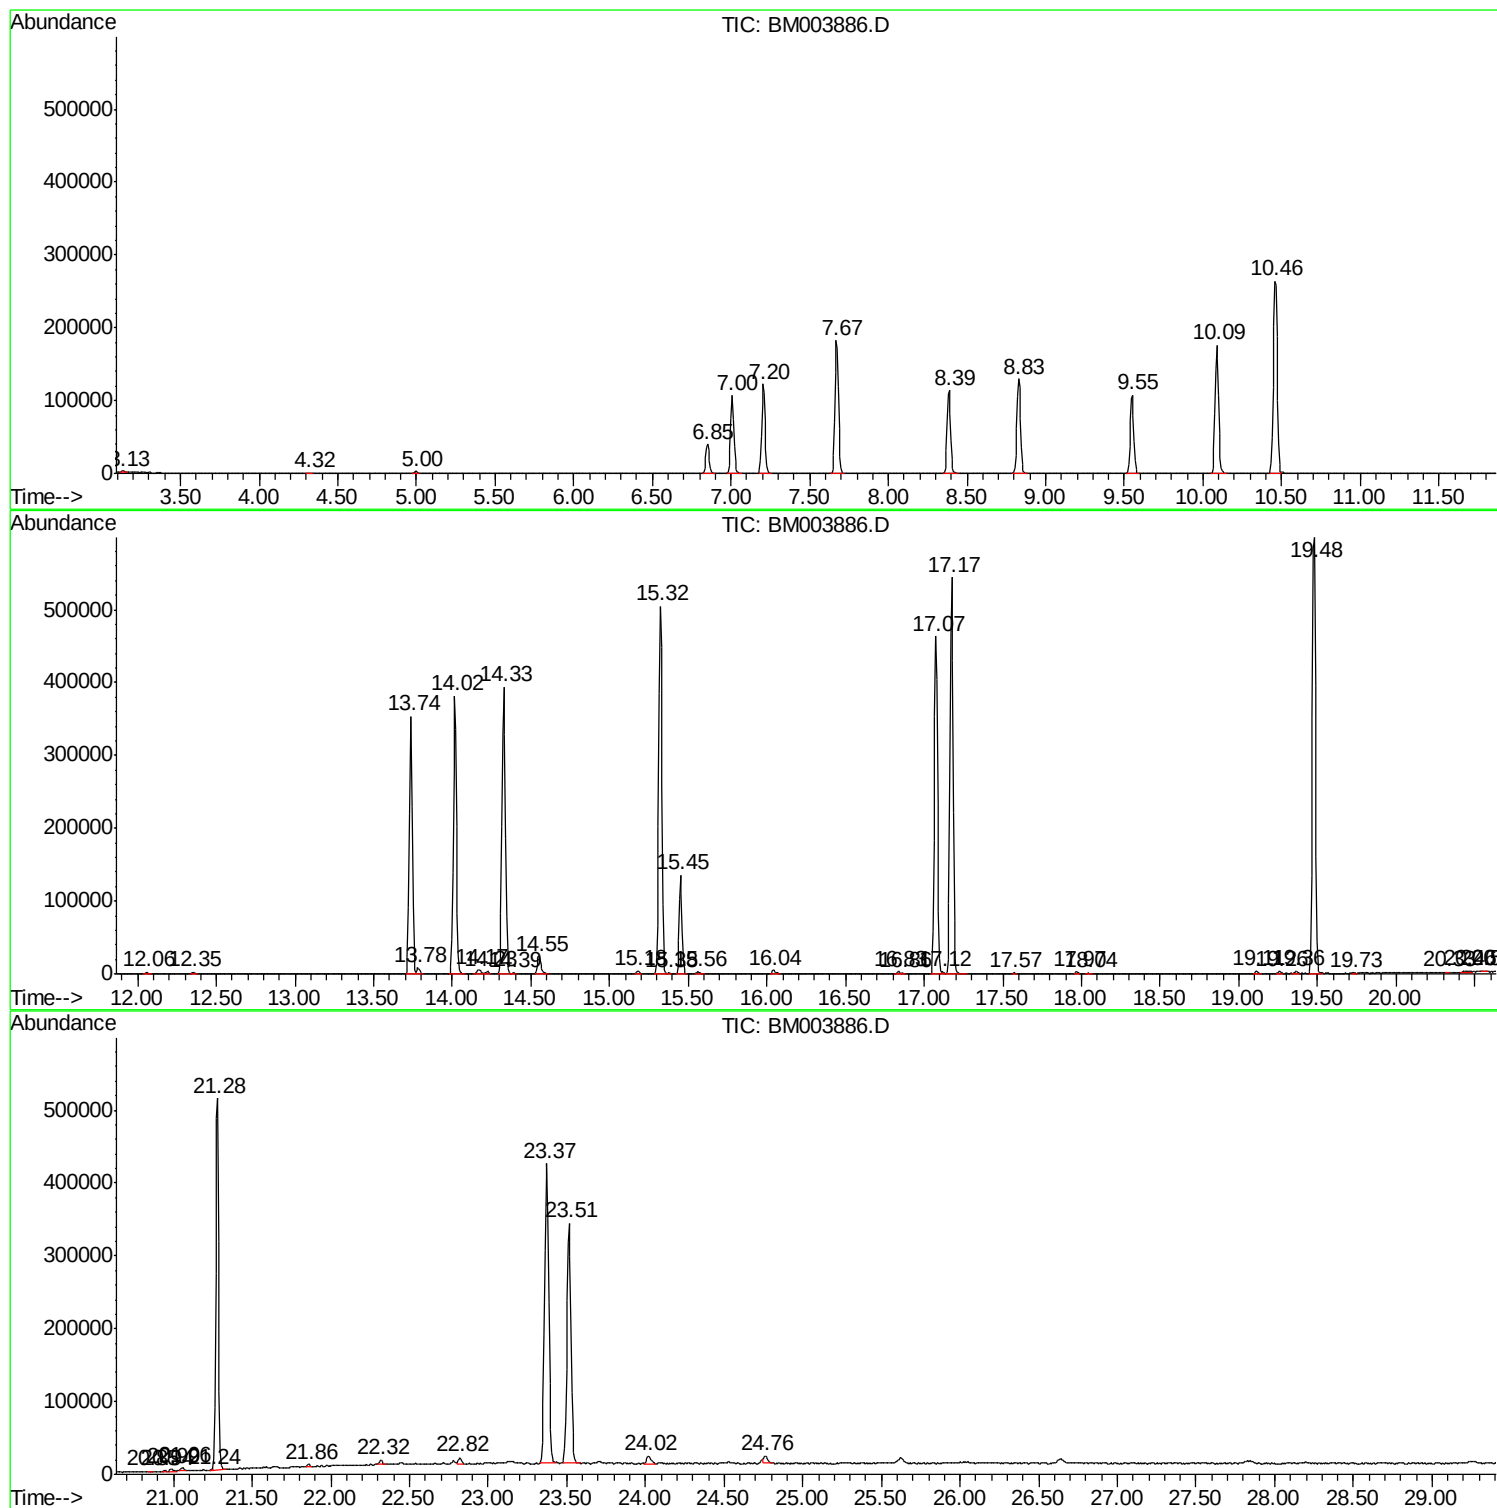

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003886.D
Acq On : 30 Dec 2015 18:53
Operator : SJ/UM
Sample : G4868-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003886.D
Acq On : 30 Dec 2015 18:53
Operator : SJ/UM
Sample : G4868-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43M8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc