

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003891.D
 Acq On : 30 Dec 2015 21:53
 Operator : SJ/UM
 Sample : G4868-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43N1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	11	rBV	2085	2375	0.19%	0.020%
2	3.169	11	14	19	rVB	4312	4976	0.41%	0.043%
3	3.875	131	134	136	rVB	1113	1256	0.10%	0.011%
4	6.851	635	640	648	rBB	49263	72531	5.92%	0.623%
5	7.004	661	666	676	rBB	154226	241649	19.73%	2.075%
6	7.204	694	700	710	rBB	175687	268527	21.93%	2.306%
7	7.669	773	779	787	rBV	180339	281488	22.99%	2.417%
8	7.733	787	790	794	rVB	5065	6305	0.51%	0.054%
9	8.039	839	842	846	rBB	2106	2567	0.21%	0.022%
10	8.386	895	901	910	rBB	153572	238248	19.46%	2.046%
11	8.828	970	976	986	rBB	191168	301695	24.64%	2.590%
12	9.551	1093	1099	1106	rBB	158618	256165	20.92%	2.199%
13	10.086	1184	1190	1202	rBB	265441	429576	35.08%	3.688%
14	10.457	1246	1253	1259	rBV	263830	434180	35.46%	3.728%
15	10.510	1259	1262	1267	rVB2	10543	15328	1.25%	0.132%
16	10.604	1273	1278	1286	rBB	11326	17140	1.40%	0.147%
17	11.374	1405	1409	1414	rBB	4322	6782	0.55%	0.058%
18	12.057	1521	1525	1529	rBB	2701	3951	0.32%	0.034%
19	12.133	1534	1538	1541	rBB	1960	2534	0.21%	0.022%
20	13.739	1804	1811	1820	rBB	522156	725498	59.25%	6.229%
21	14.015	1852	1858	1874	rVB	567070	831008	67.86%	7.135%
22	14.168	1878	1884	1889	rBV	7146	13381	1.09%	0.115%
23	14.327	1905	1911	1918	rBB2	364982	549764	44.90%	4.720%
24	14.551	1944	1949	1960	rBB	35635	57490	4.69%	0.494%
25	15.321	2074	2080	2088	rBB	756055	1062291	86.75%	9.121%
26	15.451	2097	2102	2110	rBB	231592	294132	24.02%	2.525%
27	15.562	2117	2121	2125	rBB2	5925	7108	0.58%	0.061%
28	16.868	2339	2343	2345	rBB	1239	1430	0.12%	0.012%
29	17.074	2372	2378	2384	rBV2	436401	587904	48.01%	5.048%
30	17.174	2389	2395	2405	rVV	812886	1122793	91.69%	9.640%
31	17.962	2527	2529	2534	rBV	1973	2529	0.21%	0.022%
32	18.262	2575	2580	2586	rBV2	2217	3673	0.30%	0.032%
33	18.509	2619	2622	2625	rBV2	979	1547	0.13%	0.013%
34	18.545	2625	2628	2631	rVB3	775	1238	0.10%	0.011%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003891.D
 Acq On : 30 Dec 2015 21:53
 Operator : SJ/UM
 Sample : G4868-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43N1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

35	18.686	2650	2652	2656	rVB3	1267	1638	0.13%	0.014%
36	18.756	2661	2664	2667	rVV3	1038	1651	0.13%	0.014%
37	18.897	2686	2688	2689	rBV	1459	1392	0.11%	0.012%
38	19.115	2721	2725	2728	rVV2	6453	8531	0.70%	0.073%
39	19.256	2743	2749	2753	rBV3	3041	5682	0.46%	0.049%
40	19.286	2753	2754	2757	rBV3	1234	1522	0.12%	0.013%
41	19.339	2759	2763	2764	rBV4	1032	1225	0.10%	0.011%
42	19.368	2764	2768	2772	rBV	6005	6859	0.56%	0.059%
43	19.397	2772	2773	2778	rVB3	1709	1810	0.15%	0.016%
44	19.480	2781	2787	2793	rBV	908702	1224549	100.00%	10.514%
45	19.715	2824	2827	2831	rBV	6961	7207	0.59%	0.062%
46	19.892	2854	2857	2861	rVV2	3376	3974	0.32%	0.034%
47	20.027	2876	2880	2885	rVB6	2496	3324	0.27%	0.029%
48	20.380	2937	2940	2943	rBV3	2019	2468	0.20%	0.021%
49	20.409	2943	2945	2949	rVB4	2007	2317	0.19%	0.020%
50	20.527	2961	2965	2968	rBV3	3409	5480	0.45%	0.047%
51	20.633	2979	2983	2987	rVB	12431	12048	0.98%	0.103%
52	20.991	3040	3044	3050	rVB6	5479	9084	0.74%	0.078%
53	21.056	3052	3055	3061	rVB	6408	8689	0.71%	0.075%
54	21.191	3075	3078	3081	rBV	3916	5794	0.47%	0.050%
55	21.274	3088	3092	3098	rBV	468430	615962	50.30%	5.289%
56	21.421	3115	3117	3120	rVB2	4505	4123	0.34%	0.035%
57	22.315	3266	3269	3276	rVB2	10870	13648	1.11%	0.117%
58	22.774	3345	3347	3351	rBV2	5548	7309	0.60%	0.063%
59	22.821	3351	3355	3360	rVB	13293	20915	1.71%	0.180%
60	23.374	3441	3449	3458	rBV	648621	1177718	96.18%	10.112%
61	23.515	3465	3473	3482	rBV2	314263	582098	47.54%	4.998%
62	24.021	3554	3559	3566	rVB	15887	28185	2.30%	0.242%
63	24.756	3680	3684	3692	rVB	15934	32431	2.65%	0.278%


Sum of corrected areas: 11646692

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003891.D
Acq On : 30 Dec 2015 21:53
Operator : SJ/UM
Sample : G4868-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N1

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

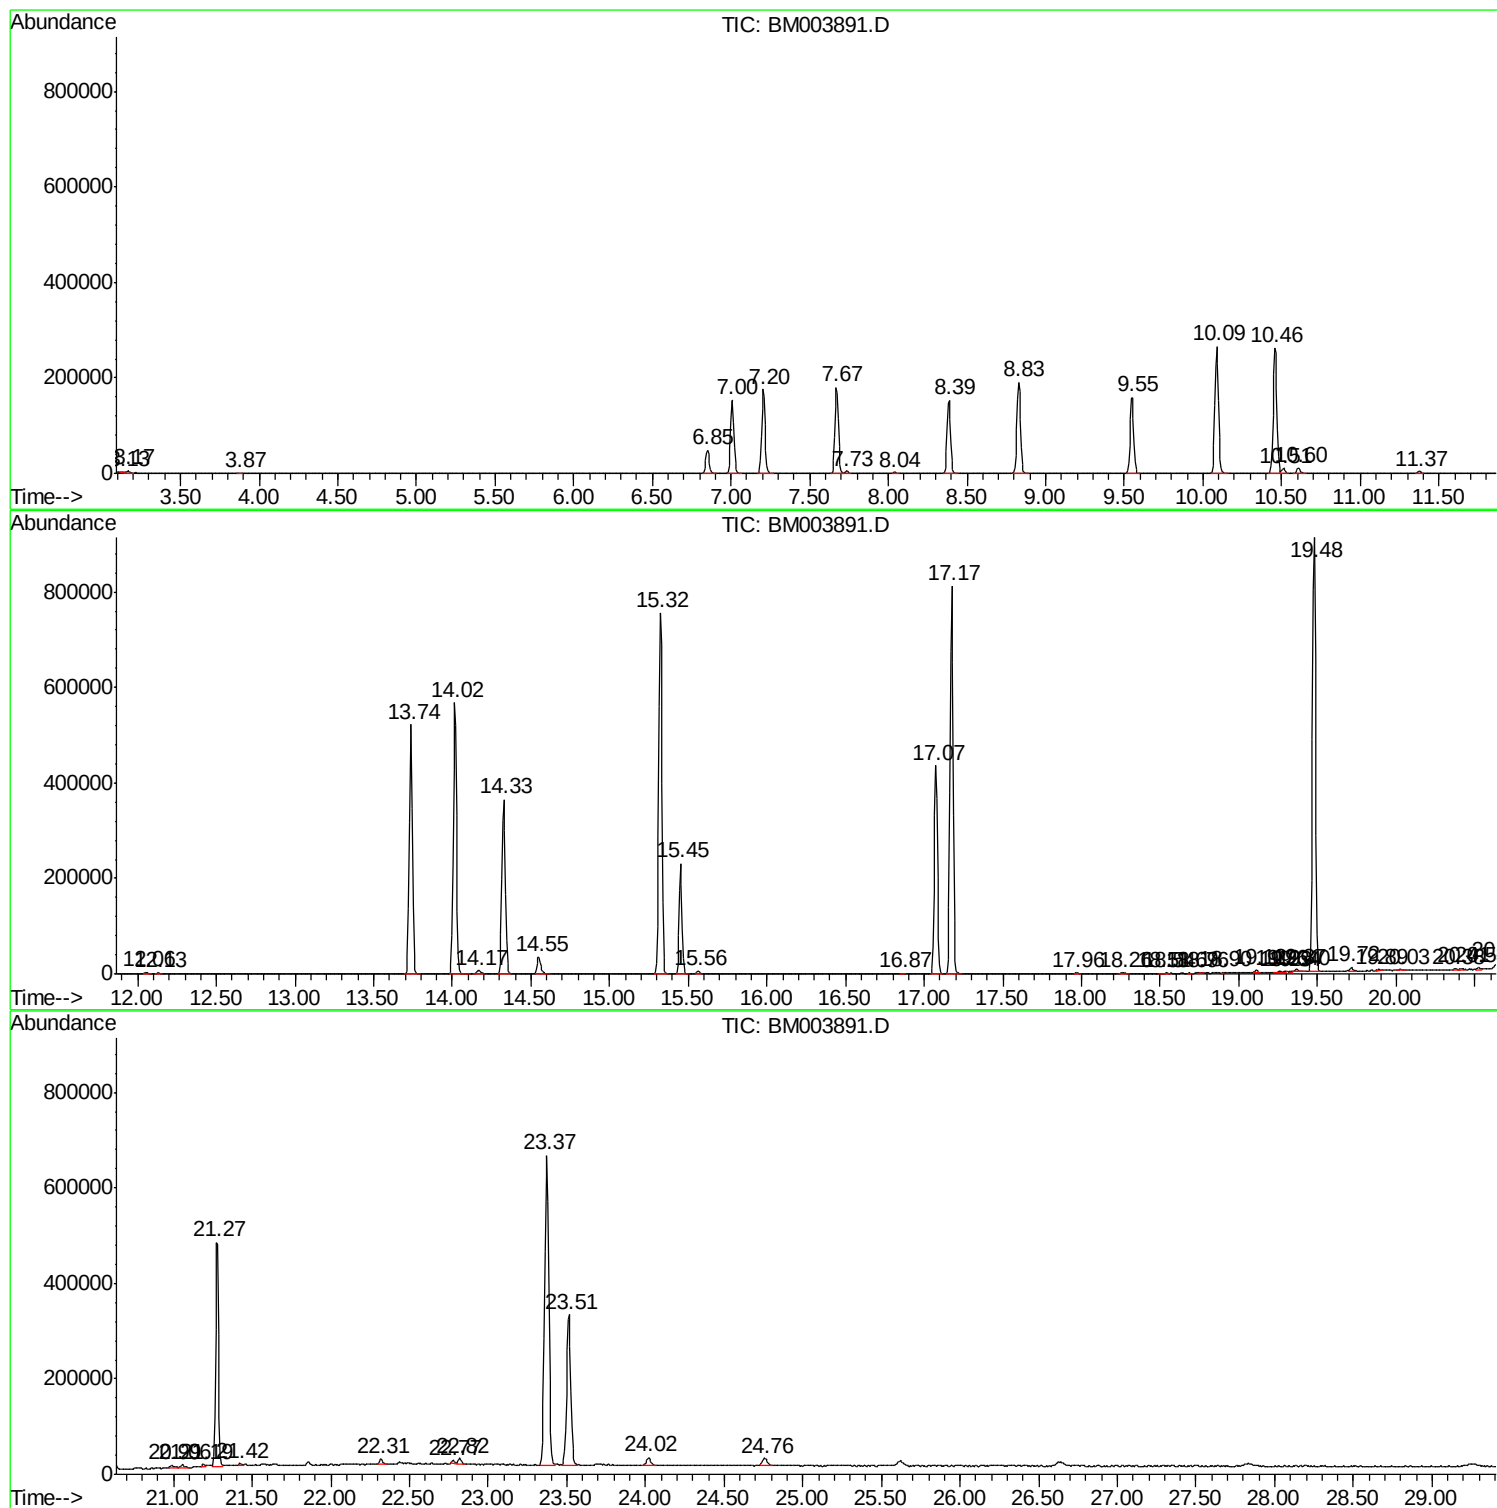

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003891.D
Acq On : 30 Dec 2015 21:53
Operator : SJ/UM
Sample : G4868-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003891.D
Acq On : 30 Dec 2015 21:53
Operator : SJ/UM
Sample : G4868-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc